



Study Data Tabulation Model Implementation Guide for Medical Devices (SDTMIG-MD)

Prepared by the
CDISC Device Team

Notes to Readers

This provisional implementation guide for medical devices corresponds to Version 1.4 of the CDISC Study Data Tabulation Model.

See Appendix E for Representation and Warranties, Limitations of Liability, and Disclaimers.

Revision History

Date	Version	Summary of Changes
January 23, 2012	1.0 Draft	Released version for public comment.
December 4, 2012	1.0 Provisional	Provisional SDTMIG-MD. Released version reflecting all changes and correction identified during the comment period.

TABLE OF CONTENTS

1	INTRODUCTION.....	1
1.1	PURPOSE	1
1.2	ORGANIZATION OF THIS DOCUMENT	2
1.3	RELATIONSHIP TO PRIOR DOCUMENTS.....	2
1.4	GENERAL NOTES AND DEFINITIONS	3
1.4.1	Electronic Submission	3
1.4.2	Differences Between Drug and Device Terminology.....	3
2	NEW SDTM-BASED DEVICE DOMAINS.....	4
2.1	OVERVIEW.....	4
2.2	NEW DOMAIN DESCRIPTIONS	4
2.3	THE OBSERVATION CLASSES OF THE DEVICE DOMAINS	5
2.4	HOW DEVICE DOMAINS RELATE TO EXISTING DOMAINS IN THE SDTMIG.....	6
2.5	HOW DEVICE DOMAINS RELATE TO EACH OTHER.....	6
3	ADDITIONS TO THE STUDY DATA TABULATION MODEL.....	12
3.1	ADDITIONS AND MODIFICATIONS TO SECTION 2.2.4, IDENTIFIERS FOR ALL CLASSES.....	12
3.2	ADDITIONS AND MODIFICATIONS TO SECTION 2.2.2, THE EVENTS OBSERVATION CLASS ..	12
4	DEVICE DOMAINS.....	13
4.1	DEVICE IDENTIFIERS - DI.....	13
4.1.1	Assumptions for the Device Identifiers Domain Model	14
4.1.2	Examples for the Device Identifiers Domain Model	17
4.2	DEVICE IN-USE - DU	19
4.2.1	Assumptions for the Device In-Use Domain Model.....	21
4.2.2	Examples for the Device In-Use Domain Model.....	22
4.3	DEVICE EXPOSURE - DX.....	24
4.3.1	Assumptions for the Device Exposure Domain Model	26
4.3.2	Examples for the Device Exposure Domain Model	27
4.4	DEVICE EVENTS - DE	30
4.4.1	Assumptions for the Device Events Domain Model.....	32
4.4.2	Examples for the Device Events Domain Model.....	33
4.5	DEVICE TRACKING AND DISPOSITION - DT	35
4.5.1	Assumptions for the Device Tracking and Disposition Domain Model	36
4.5.2	Examples for the Device Tracking and Disposition Domain Model	37
4.6	DEVICE-SUBJECT RELATIONSHIPS - DR.....	40
4.6.1	Assumptions for the Device-Subject Relationships Domain Model.....	40
4.6.2	Examples for the Device-Subject Relationships Domain Model.....	41
4.7	DEVICE PROPERTIES - DO.....	43
4.7.1	Assumptions for the Device Properties Domain Model	44
4.7.2	Examples for the Device Properties Domain Model	45
5	CROSS-DOMAIN RELATIONSHIP EXAMPLES.....	46
5.1	DEVICE IN-USE AND TEST RESULTS	46
6	APPENDICES.....	51
	Appendix A: Glossary, Acronyms, and Definitions	52
	Appendix B: Supplemental Information.....	55
	Appendix C: Other Relevant Standards.....	56
	Appendix D: Participating Companies	57
	Appendix E: Representations and Warranties, Limitations of Liability, and Disclaimers	58

1 INTRODUCTION

1.1 PURPOSE

This provisional Medical Device Implementation Guide (IG) to the Study Data Tabulation Model (SDTM) defines recommended standards for the submission of data from clinical trials in which medical devices were used, and is referred to as the SDTMIG-MD. This Implementation Guide is based on the original Study Data Tabulation Model Implementation Guide (SDTMIG) developed for human clinical trials. The device standards are intended to cover both paper and electronic regulatory submissions. Here, “electronic” means submissions that provide study and other data in machine-readable electronic database format.

Devices are an important and growing part of the medical world, both on their own and in combination with drugs or biologic agents. The ISO 14155 Medical Devices Good Clinical Practices standard defines a “device” as:

Any instrument, apparatus, appliance, material or other article, whether used alone or in combination, including the software necessary for its proper application, intended by the manufacturer to be used on human beings for the purpose of:

- *diagnosis, prevention, monitoring, treatment or alleviation of disease,*
- *diagnosis, monitoring, treatment, alleviation or compensation for an injury or handicap,*
- *investigation, replacement or modification of the anatomy or of a physiological process,*
- *control of conception,*
- *and which does not achieve its principal intended action in or on the human body by pharmacological, immunological or metabolic means, but which may be assisted in its function by such means.*

While different types of devices do have widely varying data requirements, most Class II and III devices requiring regulatory data submissions share some fundamental characteristics. This document contains Study Data Tabulation Model Implementation Guide (SDTMIG) regulatory data submission standards for some key data shared by most types of devices. It is intended to guide the organization, structure, and format of standard device clinical trial tabulation datasets submitted to regulatory authorities. This document introduces new SDTM domains, showing rules and examples implementing these domains specifically for device-related data.

This document does not contain all the domains necessary for sponsors to implement CDISC SDTM-based standards for medical device studies. Specifically, this document does not discuss existing domains that may be common to both device and drug studies, for example, Adverse Events and Demographics. These can be found in the SDTMIG (available for download at www.cdisc.org/standards). In addition, the domains defined in this Implementation Guide are not necessarily required; sponsors should use those domains that represent the data necessary to address the appropriate scientific and regulatory needs.

The domains defined in this document comprise some of the device-specific data that may be needed for the clinical sections of a regulatory submission involving devices under study. Data may be required either to answer protocol questions, to address associated safety questions, or to associate specific devices to subjects. Some data are collected on Case Report Forms that are completed by the investigative sites, while other data are usually derived by sponsors for the SDTM-based datasets. Other data needed for the submission, such as manufacturing quality information, may be included in other sections of the submission, but are not considered clinical data, and therefore are not included in the SDTM-based domains. The device domains include some non-subject data definitions, such as Device Events and Device Tracking information.

The domains in this document may also be used for studies where devices are used to obtain study measurements or results, but the devices themselves are not the object of the study. For example, a study that uses an MRI to capture images of the brain to measure brain volume for an Alzheimer's trial may

choose to use the Device In-Use domain to capture the field strength and slice thickness setting for each image, even though the MRI machine is not being studied and is already approved for use. The domains used in these circumstances will be determined by the sponsor based on the data needed for submission.

1.2 ORGANIZATION OF THIS DOCUMENT

This document contains information on how to format tabulation data for the purpose of submission. While the document is self-contained with respect to device-specific information, it has been developed to be harmonized with other CDISC standards.

This document has been organized into the following sections:

- **Section 1: Introduction** - This section provides an orientation to data submitted for medical devices.
- **Section 2: New SDTM Device Domains** - Provides an overview of the new device domains and their relationship to each other as well as to existing domains described in the SDTMIG.
- **Section 3: Proposed Additions to the Study Data Tabulation Model** - Describes proposed new variables needed to be added to the SDTM for implementation in device domains.
- **Section 4: Device Domains** - Describes each of the new device domains, including domain models, assumptions, and examples.
- **Section 5: Cross-Domain Relationship Examples** - This section describes the relationship between Device In-Use and results generated from the measurement or output of the device. It illustrates how domains can be linked.
- **Section 6: Glossary, Acronyms, and Definitions** - This section provides information on common terms, acronyms and definitions.
- **Appendices** - This section provides additional supplemental material regarding the Medical Devices project as well as references and supplemental information relevant to implementation of the Medical Devices Implementation Guide.

1.3 RELATIONSHIP TO PRIOR DOCUMENTS

This document is not intended to replace the standards defined in the current Study Data Tabulation Model Implementation Guide. This Medical Device Implementation Guide (SDTMIG-MD) should be implemented together with the SDTMIG (available at <http://www.cdisc.org/standards>). The SDTMIG is based on the general SDTM conceptual model for representing data to be submitted to regulatory authorities. The SDTM and SDTMIG should be read prior to reading the Device Implementation Guide. An understanding of both of these documents is needed before attempting to understand this Device Implementation Guide. The version used (and whether to update to newer version if relevant) is the sponsor's decision, based upon public and private communications from the FDA.

The sections of the SDTMIG that will be the most relevant are:

Section 2: Fundamentals of the SDTM

Section 4: Assumptions for Domain Models (review the introductory paragraphs in the main sections and scan the remainder)

Section 5: Models for Special-Purpose Domains (review the introductory paragraphs for each domain and scan the remainder)

Section 6: Domain Models Based on the General Observation Classes (introductory paragraphs for each domain and scan the included variables)

Section 8: Representing Relationships and Data (introductory paragraphs to the main sections, and scan the remainder to know what is included)

Appendix C: Controlled Terminology (introductory paragraphs and scan the remainder to know what is there)

1.4 GENERAL NOTES AND DEFINITIONS

1.4.1 Electronic Submission

Different segments of the drug/biologics/devices industry have different underlying assumptions with respect to submitting data to the regulatory authorities. Electronic Data refers to the practice of sending study data to a regulatory agency in an electronic format such as a dataset. In this type of submission, documents are submitted in electronic files such as MS Word, and subject and device data from clinical trials are submitted as electronic datasets using a defined data format. The following considerations might be useful to sponsors submitting data in an electronic format:

- **Paper vs. Electronic Regulatory Submission:** These standards are intended to be applicable for regulatory submissions regardless of whether the data are sent on paper, in electronic document files, or as electronic study data databases.
- **Paper CRFs vs. Electronic CRFs:** The term “CRF” used throughout this document refers to both paper and electronic formats, unless otherwise specified.
- **Fields vs. Variables:** The term data collection “fields” refers to questions that are seen on the CRF (i.e., the concept of the information solicited by a question). The term data collection “variables” refers to how data are organized and stored in a clinical database.
- **Mechanisms for Data Collection:** Different data collection mechanisms can be used to control how data are collected (e.g., tick boxes, check boxes, radio buttons, drop-down lists). For the purposes of this document, these terms will be used interchangeably. This SDTMIG-MD is designed to accommodate both paper and electronic data capture, although it does assume that data will be entered into an electronic database at some point.
- **Ancillary:** An ancillary device is one that is used in a study but is not the device under study. Information may or may not be captured for ancillary devices.

1.4.2 Differences Between Drug and Device Terminology

Differences exist between drugs and devices in the implementation of specific domains. For example, the terms Accountability, Disposition, and Exposure are used somewhat differently. Currently, many CDISC definitions are aligned with those of the drug sector. Table 1 illustrates the different uses of these terms.

Table 1: Comparison and Contrast in Term Usage in Drug vs. Device Trials

Term	Device Definition	Drug Definition
Accountability	<u>Device Accountability:</u> Tracking where the device is physically; shipping information may be on the CRF; usually between sponsor and site.	<u>Drug Accountability:</u> Tracking where the drug is; accounting for all of the drug (e.g., pill counts); in the clinical trial, usually between the site and the subject; shipping info not usually captured on CRFs.
Disposition	<u>Device Disposition:</u> The final location/status of the device at the time of submission or the end of the trial.	<u>Subject Disposition:</u> The status of the subject’s participation in the trial at a given time point (e.g., did they complete the study or withdraw early).
Exposure	<u>Device Exposure:</u> The interaction or interface between the subject and the device or device constituents. Note that exposure information about a drug delivered via a device would generally be placed in Study Drug Exposure (EX). Sponsors should confer with the regulatory reviewers to determine the correct domain to use.	<u>Study Drug Exposure:</u> The amount of study drug to which the subject is exposed.

2 NEW SDTM-BASED DEVICE DOMAINS

2.1 OVERVIEW

This Implementation Guide includes five new SDTM Device domains based on the SDTM Events, Findings, and Interventions general observation classes, and two new special-purpose domains. These domains will accommodate most of the core requirements for the majority of studies with implantable, diagnostic, and imaging devices. When CDASH models are developed, they will be presented in both normalized and non-normalized (tall and narrow) layouts. Users may employ whichever structure is optimal for them for data capture.

Medical Device domains are somewhat different from many other SDTM domains developed thus far in that they may capture information about entities other than the study subject or the trial itself. They must also accommodate a more complex set of data, and more variation in the relationship of the device to subjects, than that in typical drug development studies. As a result, developing a relationship structure that is not typically required in most subject-related data (e.g., Device-Subject Relationships domain) was required.

2.2 NEW DOMAIN DESCRIPTIONS

The following seven new SDTM-based domains are included in this Implementation Guide:

1. Study Device Identifiers (DI): This is a special-purpose domain designed for the submission of information that identifies a specific device unit. The primary purpose of this domain is to provide a consistent sponsor-defined variable (SPDEVID) for linking data across Device domains, independent of the level of granularity by which a device might be identified by a sponsor in a study. The information included in Study DI depends upon what is needed to identify the device uniquely within a submission and to meet analysis and regulatory requirements. The domain is not intended to contain information about characteristics that can change without affecting the identification of the device, such as supplier details or dial settings (e.g., imaging devices). Device Identifiers exist independently from subjects and therefore the Study DI domain does not contain USUBJID.
2. Device In-Use (DU): Device In-Use is a Findings domain that contains the values of measurements and settings that are intentionally set on a device when it is used, and may vary from subject to subject or other target. These are characteristics that exist for the device, and have a specific setting for a use instance. DU is distinct from Device Properties, which describes static characteristics of the device. For example: Device Properties would capture that an MRI machine's field strength has a range from 0.2 to 3 Tesla, whereas the Device In-Use domain would capture that the field strength for the MRI scan for Subject 123 was 0.5 T.
3. Device Exposure (DX): Device Exposure is an Interventions domain that records the details of a subject's exposure to a medical device under study. This device is prospectively defined as a test article within a study and may be used by the subject, on the subject, or be implanted into the subject. Examples include but are not limited to stents, drug delivery systems, and any other item under study that is defined as a device in the applicable regulations.
4. Device Events (DE): DE is an Events domain that contains information about various kinds of device-related events, such as device malfunctions. A device event may or may not be associated with a subject or a visit. If a device event, such as a malfunction, results in an adverse event, then the AE-related information should be recorded in the Adverse Events (AE) domain (see SDTMIG, AE domain). The relationship between the AE and a device malfunction in DE can be recorded using RELREC (see SDTMIG section "Relating Datasets") and appropriate identifying variables such as DESPID and AESPID.
5. Device Tracking and Disposition (DT): The Device Tracking and Disposition domain is an Events domain that represents a record of tracking events for a given device. This could include initial shipment, deployment, return, destruction, etc. Different events would be relevant to different types of devices. The last record represents the device disposition at the time of submission. The sponsor

- decides upon the level of granularity that is appropriate for this domain based on the type of device and agreements with the regulatory agencies.
6. Device-Subject Relationships (DR): The Device-Subject Relationships domain is a special-purpose domain that links each subject to devices to which they may have been exposed. Information in this table may have been initially collected and submitted in other domains (e.g., Device Exposure, Device Tracking and Disposition, Device Events). This domain, however, provides a single, consistent location to find the relationship between a subject and a device, regardless of the device or the domain in which subject-related data may have been collected or submitted.
 7. Device Properties (DO): The Device Properties Findings domain is used to report characteristics of the device that are important to include in the submission, do not vary over the course of the study but are not used to identify the device. Examples include expiration date or shelf life. Device Properties exist independently from subjects and therefore the DO domain does not contain USUBJID.

Although some domains, such as Device In-Use, were developed to support submission of device-related data in both device and non-device-focused trials (e.g., where the device is used to generate study measurements and is not itself under study), any of these domains can be used in any trial type, including device/drug and device/biologic combination trials, if deemed appropriate by the sponsor and regulators.

2.3 THE OBSERVATION CLASSES OF THE DEVICE DOMAINS

The following list shows the observation class for each device domain.

Special-Purpose Domains

- Device Identifiers - DI
- Device-Subject Relationships - DR

Interventions General Observation Class

- Device Exposure - DX

Events General Observation Class

- Device Events - DE
- Device Tracking - DT


Findings General Observation Class

- Device-In-Use - DU
- Device Properties - DO

2.4 HOW DEVICE DOMAINS RELATE TO EXISTING DOMAINS IN THE SDTMIG

Figure 1 illustrates new and existing SDTM-based domains, and the combinations of subject and/or device data they might contain. The domains listed below are only examples of those that might or might not contain device and/or subject data.

Figure 1. Device and Subject Data in Different Domains

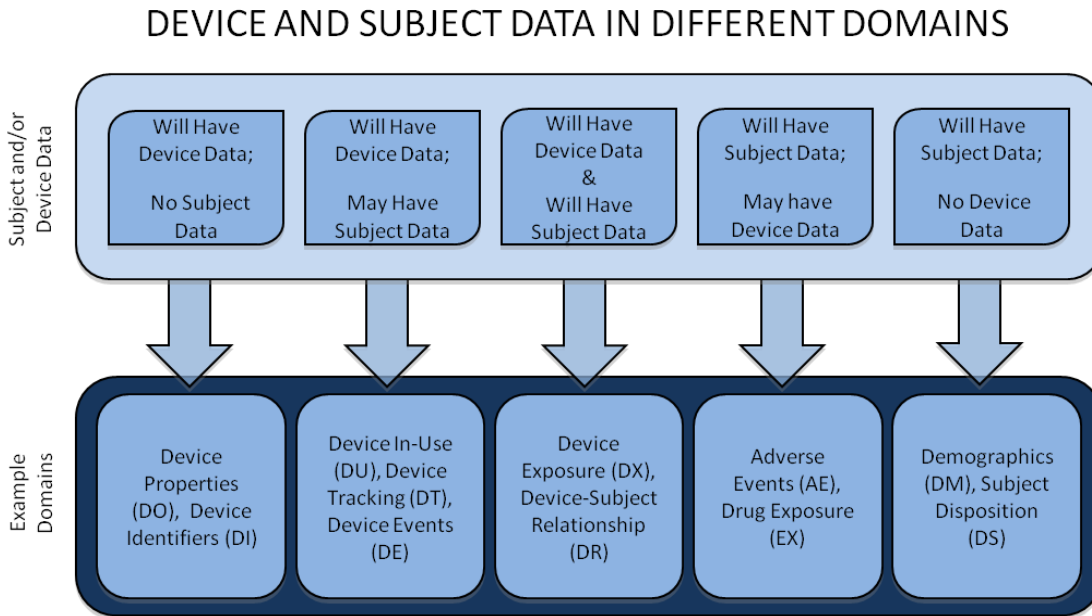

2.5 HOW DEVICE DOMAINS RELATE TO EACH OTHER

Figures 2a-2f show examples of how the different domains relate to each other through the choice of identifiers present in each. In these examples, Subject 02-1024 in Study ABC-123 had one telescoping titanium orthopedic rod implanted. The rod was sourced from Rods, Co. (DI) and has a length of 4 cm when fully contracted and 8 cm when fully extended (DO). The sponsor would decide whether to model the lengths separately in DO as minimum and maximum lengths, or as a single size characteristic. Here the sizes are separated.

The model name is SuperLynx (DI), and the serial number for the rod is 274962 (DI). These, plus the manufacturer, are the only characteristics needed to identify each rod uniquely. This domain associates the three key identifier characteristics to the single SPDEVID (TEL-3745), used to reference the device across the other domains. The fourth record in DI is the TYPE, which is required for all device submissions where any device-specific information is included, and is encouraged for the remainder. For post-marketing studies, the use of FDAUDI (the FDA’s UDI identifier) is also required, but this example represents a pre-approval study.

The rod was shipped from the sponsor to Site 02 on 26Apr2011 (DT), and implanted into the subject on 29Apr2011 (DT & DX). When implanted, the telescoping length was set to 4 cm (DU). The rod was implanted into the right femur (DX). There were no malfunctions or other events (no DE), and the device was not explanted (no explantation record in DT and no end date in DX). In this case, the relationship between the device and the subject is derived from DX into DR. The purpose of DR is to provide a link between device and subject data independent of the identifiers that exist on each domain, or of the domains that are present for a given submission.

The different identifiers (study, subject, and device) are color and pattern coded in the data tables below to facilitate identifying the relationships of the data between the domains and to see how different domains use different combinations of identifiers. Note that, in order to simplify the display, the tables contain a subset of the available variables.

Figures 2a-2f. How Device Domains Relate to Each Other - Simple Examples

Figure 2a. Study Device Identifiers using Study ID and Sponsor Device ID only.

(Study) Device Identifiers (DI)				
STUDYID	SPDEVID	DIPARMCD	DIPARM	DIVAL
<i>Study Identifier</i>	<i>Sponsor Device Identifier</i>	<i>Device Identifier Element Short Name</i>	<i>Device Identifier Element Name</i>	<i>Device Identifier Element Value</i>
ABC-123	TEL-3745	MANUF	Manufacturer	Rods, Co.
ABC-123	TEL-3745	MODEL	Model	SuperLynx
ABC-123	TEL-3745	SERIAL	Serial Number	274962
ABC-123	TEL-3745	TYPE	Type of device	Telescoping orthopedic rod

Figure 2b. Device Properties using Study ID and Sponsor Device ID only.

Device Properties (DO)						
STUDY ID	USUBJID	SPDEVID	DOTESTCD	DOTEST	DOORRES	DOORRESU
<i>Study Identifier</i>	<i>Unique Subject Identifier</i>	<i>Sponsor Device Identifier</i>	<i>Device Property Short Name</i>	<i>Device Property Test Name</i>	<i>Result or Finding in Original Units</i>	<i>Original Units</i>
ABC-123	02-1024	TEL-3745	COMPOS	Composition	Titanium	
ABC-123	02-1024	TEL-3745	MXLENGTH	Maximum Length	8	cm
ABC-123	02-1024	TEL-3745	MNLENGTH	Minimum Length	4	cm

Figure 2c. Device Exposure using Study ID, Subject ID, and Sponsor Device ID.

Device Exposure (DX)							
STUDYID	USUBJID	SPDEVID	DXTRT	DXLOC	DXLAT	DXSTDTC	DXENDTC
<i>Study Identifier</i>	<i>Unique Subject Identifier</i>	<i>Sponsor Device Identifier</i>	<i>Name of Device Exposure or Output</i>	<i>Location of Device Exposure</i>	<i>Laterality of Device Exposure</i>	<i>Start Date/Time of Device Exposure</i>	<i>End Date/Time of Device Exposure</i>
ABC-123	02-1024	TEL-3745	SuperLynx Ortho Rod	FEMUR	RIGHT	2011-04-29	(null)

Figure 2d. Device In-Use using Study ID, Subject ID, and Sponsor Device ID.

Device –In-Use (DU)							
STUDY ID	USUBJID	SPDEVID	DUTESTCD	DUTEST	DUORRES	DUORRES U	DUDTC
<i>Study Identifier</i>	<i>Unique Subject Identifier</i>	<i>Sponsor Device Identifier</i>	<i>Device In-Use Test Short Name</i>	<i>Device In-Use Test Name</i>	<i>Result or Finding in Original Units</i>	<i>Original Units</i>	<i>Date/Time Device Used With Test/ Setting</i>
ABC-123	02-1024	TEL-3745	ISLENGTH	In situ length	4	cm	2011-04-29

Figure 2e. Device Tracking using Study ID and Device ID only. When the subject appears, it is as a value of DTPARTY / DTPRTYID.

Device Tracking & Disposition (DT)					
STUDYID	SPDEVID	DTTERM	DTPARTY	DTPRTYID	DTSTDTC
<i>Study Identifier</i>	<i>Sponsor Device Identifier</i>	<i>Reported Term for the Tracking Event</i>	<i>Party Responsible for the Device</i>	<i>Responsible Party Identifier</i>	<i>Start Date/Time of Device Tracking Event</i>
ABC-123	TEL-3745	SHIPPED	SITE	02	2011-04-26
ABC-123	TEL-3745	IMPLANTED	SUBJECT	02-1024	2011-04-29

Figure 2f. Device-Subject Relationship using Study ID, Subject ID and Sponsor Device ID.

Device-Subject Relationship (DR)		
STUDYID	USUBJID	SPDEVID
<i>Study Identifier</i>	<i>Unique Subject Identifier</i>	<i>Sponsor Device ID</i>
ABC-258	04-1027	TEL-8526

Figures 3a-3i show more complex examples of domain relationships. In Study ABC-258, Subject 04-1027 had a telescopic titanium orthopedic rod implanted. The rod’s maximum extended length is 8 cm, its minimum length is 4 cm, and the rod’s composition is of titanium (DO). The test device’s manufacturer (Rods, Co.) appears in DI, along with the model (SuperLynx) and serial number (562987) to ensure uniqueness. In this case, there is a comparator device (not shown), and similar information would be added for the comparator device. DR links device and subject data regardless of what identifiers exist.

The rod was shipped from the sponsor to Site 04 on 23May2011 (DT), and implanted into the subject on 12Jun2011 (DT & DX). It was explanted on 01Jul2011, and shipped back to the sponsor on 25Jul2011 (DT & DX). Note that the implantation and explantation data in DT is for device accountability and not for exposure. In other cases it may not mirror exposure as closely. When implanted, the telescoping length was set to 6 cm (DU).

The device developed a fissure (DE), considered a malfunction (DECAT), at which point the subject developed inflammation at the incision site (AE). This AE caused the device to be explanted (DE, and could also appear in DX) and the subject to discontinue from the study (DS). If the appropriate links are collected, the malfunction and its associated AE can be linked via RELREC records. Note that this medical

device implementation guide does not include the AE and DS domains, since they are defined in the SDTMIG.

As with the examples above in Figure 2, the different identifiers (study, subject, and device) are color and pattern coded in the data tables below to facilitate identifying the relationships of the data between the domains. Note that, in order to simplify the display, the tables contain a subset of the available variables.

Figures 3a-3i. How Device Domains Relate to Each Other - Complex Examples

Figure 3a. Study Device Identifiers using Study ID and Sponsor Device ID only.

(Study) Device Identifiers (DI)				
STUDYID	SPDEVID	DIPARMCD	DIPARM	DIVAL
<i>Study Identifier</i>	<i>Sponsor Device Identifier</i>	<i>Device Identifier Element Short Name</i>	<i>Device Identifier Element Name</i>	<i>Device Identifier Element Value</i>
ABC-258	TEL-8526	MANUF	Manufacturer	Rods, Co.
ABC-258	TEL-8526	MODEL	Model	SuperLynx
ABC-258	TEL-8526	SERIAL	Serial Number	562987
ABC-258	TEL-8526	TYPE	Type of device	Telescoping orthopedic rod

Figure 3b. Device Properties using Study ID and Sponsor Device ID only.

Device Properties (DO)						
STUDYID	USUBJID	SPDEVID	DOTESTCD	DOTEST	DOORRES	DOORRESU
<i>Study Identifier</i>	<i>Unique Subject Identifier</i>	<i>Sponsor Device Identifier</i>	<i>Device Property Short Name</i>	<i>Device Property Test Name</i>	<i>Result or Finding in Original Units</i>	<i>Original Units</i>
ABC-258	04-1027	TEL-8526	MXLENGTH	Maximum Length	8	cm
ABC-258	04-1027	TEL-8526	MNLENGTH	Minimum Length	4	cm
ABC-258	04-1027	TEL-8526	COMPOS	Composition	Titanium	

Figure 3c. Device Exposure using Study ID, Subject ID and Sponsor Device ID.

Device Exposure (DX)							
STUDYID	USUBJID	SPDEVID	DXTRT	DXLOC	DXLAT	DXSTDTC	DXENDTC
<i>Study Identifier</i>	<i>Unique Subject Identifier</i>	<i>Sponsor Device Identifier</i>	<i>Name of Device Exposure or Output</i>	<i>Location of Device Exposure</i>	<i>Laterality of Device Exposure</i>	<i>Start Date/Time of Device Exposure</i>	<i>End Date/Time of Device Exposure</i>
ABC-258	04-1027	TEL-8526	SuperLynx Ortho Rod	FEMUR	LEFT	2011-06-12	2011-07-01

Figure 3d. Device-In-Use using Study ID, Subject ID and Sponsor Device ID.

Device –In-Use (DU)							
STUDYID	USUBJID	SPDEVID	DUTESTCD	DUTEST	DUORRES	DUORRESU	DUDTC
<i>Study Identifier</i>	<i>Unique Subject Identifier</i>	<i>Sponsor Device Identifier</i>	<i>Device In-Use Test Short Name</i>	<i>Device In-Use Test Name</i>	<i>Result or Finding in Original Units</i>	<i>Original Units</i>	<i>Date/Time Device Used With Test/Setting</i>
ABC-258	04-1027	TEL-8526	ISLENGTH	In situ length	6	cm	2011-06-12

Figure 3e. Device Tracking using Study ID and Sponsor Device ID only. When the subject appears, it is as a value of DTPARTY / DTPRTYID.

Device Tracking & Disposition (DT)					
STUDYID	SPDEVID	DTTERM	DTPARTY	DTPRTYID	DTSTDTC
<i>Study Identifier</i>	<i>Sponsor Device Identifier</i>	<i>Reported Term for the Tracking Event</i>	<i>Party Responsible for the Device</i>	<i>Responsible Party Identifier</i>	<i>Start Date/Time of Device Tracking Event</i>
ABC-258	TEL-8526	SHIPPED	SITE	04	2011-05-23
ABC-258	TEL-8526	IMPLANTED	SUBJECT	04-1027	2011-06-12
ABC-258	TEL-8526	EXPLANTED	SITE	04	2011-07-01
ABC-258	TEL-8526	SHIPPED	SPONSOR		2011-07-25

Figure 3f. Device Events using Study ID, Subject ID and Sponsor Device ID.

Device Events (DE)									
STUDY ID	USUBJID	SPDEVID	DESPID	DETERM	DEDECOD	DECAT	DEACNDEV	DESTDTC	DEENDTC
<i>Study Identifier</i>	<i>Unique Subject Identifier</i>	<i>Sponsor Device Identifier</i>	<i>Sponsor-Defined Identifier</i>	<i>Reported Term for Device Event</i>	<i>Device Events Dictionary-Derived Term</i>	<i>Category of Device Event</i>	<i>Action Taken with Device</i>	<i>Start Date/Time of Device Event</i>	<i>End Date/Time of Device Event</i>
ABC-258	04-1027	TEL-8526	2	Fissure formation	FISSFORM	MALFUNCTION	Device Explanted	2011-06-25	

Figure 3g. Device-Subject Relationship using Study ID, Subject ID and Sponsor Device ID.

Device-Subject Relationship (DR)		
STUDYID	USUBJID	SPDEVID
<i>Study Identifier</i>	<i>Unique Subject Identifier</i>	<i>Sponsor Device ID</i>
ABC-258	04-1027	TEL-8526

Figure 3h. Adverse Events using Study ID and Subject ID. At the time of this publishing, the mechanism of linking the specific AE to the specific device has not yet been established. This figure shows what the data might look like in the AE domain. The linkage could be accomplished using --SPID variables in data capture and this could permit the construction of a RELREC dataset.

Adverse Events (AE)							
STUDY ID	USUBJID	AESPID	AEDECOD	AETERM	AEACNOTH	AESTDTC	AEENDTC
<i>Study ID</i>	<i>Unique Subject ID</i>	<i>Sponsor-Defined ID</i>	<i>Dictionary Derived Term</i>	<i>Event Verbatim Term</i>	<i>Other Action Taken For AE</i>	<i>Event Start Date/Time</i>	<i>Event End Date/Time</i>
ABC-258	04-1027	3	INFLAMMATION	Incision site inflammation	Device removed	2011-06-25	2011-07-10
ABC-258	04-1027	4	HEADACHE	Headache	None	2011-06-30	2011-07-02

Figure 3i. Subject Disposition Study ID and Subject ID only. The event is Discontinuation from the Study Due to an AE. The “start” date is also used for a point in time event, which is the case here. If the specific device needs to be linked to this event, it could be accomplished in data capture using --SPID variables, which can then be reflected here in a RELREC dataset.

Subject Disposition (DS)				
STUDYID	USUBJID	DSDECOD	DSTERM	DSDTDTC
<i>Study ID</i>	<i>Unique Subject ID</i>	<i>Standardized Disposition Term</i>	<i>Disposition Event Reported Term</i>	<i>Disposition Event Start Date/Time</i>
ABC-258	04-1027	ADVERSE EVENT	Adverse event	2011-07-01

3 ADDITIONS TO THE STUDY DATA TABULATION MODEL

3.1 ADDITIONS AND MODIFICATIONS TO SECTION 2.2.4, IDENTIFIERS FOR ALL CLASSES

Variable Name	Variable Label	Type	Role	Description	SDTMIG	SEND
Qualifier Variables						
SPDEVID	Sponsor Device Identifier	Char	Identifier	Sponsor-defined identifier for a device	√	

Variable order should be as follows:

SPDEVID	After USUBJID
---------	---------------

3.2 ADDITIONS AND MODIFICATIONS TO SECTION 2.2.2, THE EVENTS OBSERVATION CLASS

Variable Name	Variable Label	Type	Role	Description	SDTMIG	SEND
Qualifier Variables						
--PARTY	Accountable Party	Char	Record Qualifier	Party accountable for the device or other object as a result of the activity performed in the associated --TERM variable. The party could be an individual (e.g., subject), an organization (e.g., sponsor), or a location that is a proxy for and individual or organization (e.g., site). It is usually a somewhat general term that is further identified in the --PRTYID variable. For example, the --TERM action could be SHIPPED, the --PARTY could be SITE and the --PRTYID could be 02, signifying that the device was shipped to Site 02 and they become responsible for it.	√	
--PRTYID	Identification of specific accountable party	Char	Record Qualifier	Identification of the specific party accountable for the device after the action in --TERM is taken. Used in conjunction with --PARTY.	√	
--ACNDEV	Action Taken with Device	Char	Record Qualifier	Action taken with respect to a device in a study, which may or may not be the device under study	√	

Variable order should be as follows:

--PARTY --PRTYID	In order, after --LOC
--ACNDEV	After --ACNOTH

4 DEVICE DOMAINS

4.1 DEVICE IDENTIFIERS - DI

di.xpt, Device Identifiers - Special Purpose, Version 1.0. One record per device identifier per device, Tabulation

Variable Name	Variable Label	Type	Controlled Terms, Codelist or Format	Role	Definition	Implementation Notes	Core
STUDYID	Study Identifier	Char		Identifier	Unique identifier for a study.	Unique identifier for a study.	Req
DOMAIN	Domain Abbreviation	Char	DI	Identifier	Two-character abbreviation for the domain.	Two-character abbreviation for the domain.	Req
SPDEVID	Sponsor Device Identifier	Char		Identifier	Sponsor-defined identifier for the device.	It must be unique for each tracked unit of the device under study, and can be at whatever level of granularity the device should be identified (e.g., model or serial number, or combination of identifiers).	Req
DISEQ	Sequence Number	Num		Identifier	Sequence number given to ensure uniqueness within a parameter within a device (SPDEVID) within dataset	If there is only one value for DIPARMCD for each value of SPDEVID, then DISEQ will be 1 for all records. DISEQ must be a valid number.	Exp
DIPARMCD	Device Identifier Element Short Name	Char	*	Topic	Short name of the identifier characteristic of the device.	Examples: SERIAL, MODEL. A record with DIPARMCD = TYPE should be included (see below)	Req
DIPARM	Device Identifier Element Name	Char	*	Synonym Qualifier	Name of the identifier characteristic of the device.	Examples: Serial Number, Model. A record with DIPARM = Type should be included (see below)	Req
DIVAL	Device Identifier Element Value	Char	*	Result Qualifier	Value for the parameter.	Value for the parameter. When DIPARM = Type, DIVAL should be a value in the GMDN dictionary (see below)	Req

** Indicates variable may be subject to controlled terminology, (Parenthesis indicates CDISC/NCI code list code value)*

4.1.1 Assumptions for the Device Identifiers Domain Model

1. Device Identifiers (DI) is a special-purpose domain that provides a mechanism for using multiple identifiers to create a single identifier for each device.
2. The primary purpose of this domain is to provide a consistent variable (SPDEVID) for linking data across Device domains, independent of the level of granularity by which a device might be identified by a sponsor in a study. One of the challenges of identifying devices consistently is that different types of devices use different characteristics and different numbers of characteristics as identifiers. For example, it may be sufficient to use a serial number only to identify an MRI machine, but identifying a box of screws may require a batch number and a box number. In study-specific datasets this could be accomplished by using different numbers of identifier variables, but this is not feasible for a general standard. SPDEVID is a mechanism for aggregating any number of identifiers into one, allowing for a consistent structure for identifying all devices. SPDEVID is a surrogate identifier that represents all the characteristics of a device in the Study DI domain, but is a simple, short identifier that can appear in each dataset. Having different identifier variables in different submissions does not help interoperability, and this approach allows for a single identifier while preserving access to the identifying information needed for the submission. It also facilitates merging datasets.
3. DI was modeled as a Special Purpose domain because it has none of the characteristics (except identifiers) of a Findings domain, and is clearly not an event or intervention. This is separated from the Device Properties (DO) domain because DI contains the total set of characteristics necessary for device identification, whereas DO contains information important for submission but that are not part of the device identifier.
4. In order to determine the right level of granularity for the parameters defined in DI, it is critical that the sponsor think carefully about how the devices will need to be tracked in, for example, Device In-Use, Device Events, etc., and designs SPDEVID to reflect that level of specificity. For example, if surgical screws only need to be tracked by box and not by individual screw, then the value in SPDEVID might be a box number. If each screw needs to be tracked, then the parameters would need to include the identifier on each screw.
5. The Device Identifiers domain must exist if SPDEVID is used in any domain in a study. It is required when any device-specific information is submitted. This includes information about the device under study as well as parameters captured for devices not under study (e.g., MRI slice thickness, field strength). If none of this applies (e.g., ECG machine used to generate a tracing, but no information about the machine is needed), then DI is not required.
6. If the Device Identifiers domain exists, at a minimum it must contain a record with TYPE populated.
7. SPDEVID should not change during a specific device's lifetime.
8. TYPE uses controlled terminology defined by FDA as Global Medical Device Nomenclature (GMDN). As of the date of this publication, the GMDN is not freely available to the public. In its UDI rule, the FDA indicated that GMDN will not be a requirement unless it is available to the public at no cost.
9. DISEQ must be unique within each value of DIPARMCD within a SPDEVID. If there is only 1 value of DIPARMCD per device, then DISEQ will always be 1.
10. The DI domain was designed to be able to handle situations where SPDEVID is needed to identify individual devices. In some situations, such as studies in which a device is not the product under study and is used only to conduct assessments, SPDEVID may need only to identify a kind of device. For example, an oncology trial might need to identify the kind of device used to image a tumor, in which case SPDEVID might be used to distinguish MRI, CT, and X-Ray devices. In such cases, the minimum requirement for a SPDEVID for a kind of device is TYPE (DIPARMCD=TYPE). Sponsors should define the appropriate level of granularity for unique identification; in some cases it may be a serial number, whereas in others it may be a box, lot or batch number, or some combination of these or other identifiers.
11. The DI domain is often referred to as the Study DI domain to help distinguish it from the FDA's Unique Device Identifier.

12. This domain should not be used for device characteristics other than identifiers. Any additional non-identifier attributes that the sponsor needs to submit should be placed in Device Properties (DO) instead.
13. This structure allows for the association between one SPDEVID and as many identifiers as a sponsor feels necessary to support all the submitted data. This easily transforms into a one-record-per-SPDEVID structure for potential merging with other device-related datasets that would contain the SPDEVID variable, as shown in these samples for a set of Study DI records for a single device.

DI Data arranged vertically (normalized) showing correspondence between identifiers and SPDEVID (SDTM structure):

STUDYID	DOMAIN	SPDEVID	DISEQ	DIPARMCD	DIPARM	DIVAL
DEVM-0004-0003	DI	ABC001	1	TYPE	Device Type	STENT
DEVM-0004-0003	DI	ABC001	2	MANUF	Manufacturer	Acme Stents
DEVM-0004-0003	DI	ABC001	3	MODEL	Model	45-JFI
DEVM-0004-0003	DI	ABC001	4	BATCH	Batch identifier	2011-1307
DEVM-0004-0003	DI	ABC001	5	LOT	Lot Identifier	45678
DEVM-0004-0003	DI	ABC001	6	SERIAL	Serial Number	456789132-AXQ
DEVM-0004-0003	DI	ABC001	7	Y	Manufacturer Y-code	32110
DEVM-0004-0003	DI	ABC001	8	Z	Manufacturer Z-code	6A-55

DI data arranged horizontally (non-normalized) showing identifiers and SPDEVID on a single record (non-SDTM structure):


SPDEVID	TYPE	MANUF	MODEL	BATCH	LOT	SERIAL	IDENTIFIER Y	IDENTIFIER Z
ABC001	STENT	Acme Stents	45-JFI	2011-1307	45678	456789132-AXQ	32110	6A-55

14. The data in this domain may be derived (manually or electronically), captured on DI CRFs, or a combination of these.
15. No date variables have been included in this domain because the characteristics defined in Study DI should not change over the course of the trial and because temporal associations will generally be captured in other domains, for example, Device Exposure (DX) or Device Tracking and Disposition (DT).
16. No additional variables can be added to this dataset.
17. DIPARMCD values are limited to 8 characters and cannot begin with a number or underscore as they can be used as variable names when the dataset is transposed to a non-normalized structure.
18. If FDAUDI is used, it is intended to hold the FDA’s UDI assigned after device approval. For post-approval studies, SPDEVID could be the FDAUDI value only. If the device is pre-approval, this variable would be null.
19. If the FDAUDI can be populated, the TYPE should still be included. Sponsors may include additional parameters as needed.
20. An incomplete list of DIPARMCD and DIPARM values is shown in the following table.

DIPARMCD	DIPARM
FDAUDI	FDA Unique Device Identifier
TYPE	Device Type
MANUF	Manufacturer
MODEL	Model

BATCH	Batch identifier
LOT	Lot Identifier
SERIAL	Serial Number

21. Generally, the SPDEVID should include the set of parameters necessary for identifying the device uniquely, and would also have all of the higher level parameters. For example, if Serial Number were sufficient to identify the device, generally Model, Manufacturer and Device Type would be included (if available or relevant). The following graphic shows the usual relationships between identifier parameters. In the smallest shapes, Lot, Batch and Serial Number are usually considered to be on the same level. The FDAUDI is effectively a surrogate key for the rest of the identifiers, so the combination of FDAUDI and TYPE could be sufficient to identify each device for a postmarketing study. Alternatively, if information embedded in the FDAUDI is needed for data aggregation, analysis or appropriate interpretation of the data, other identifier variables can also be extracted from FDAUDI and included.

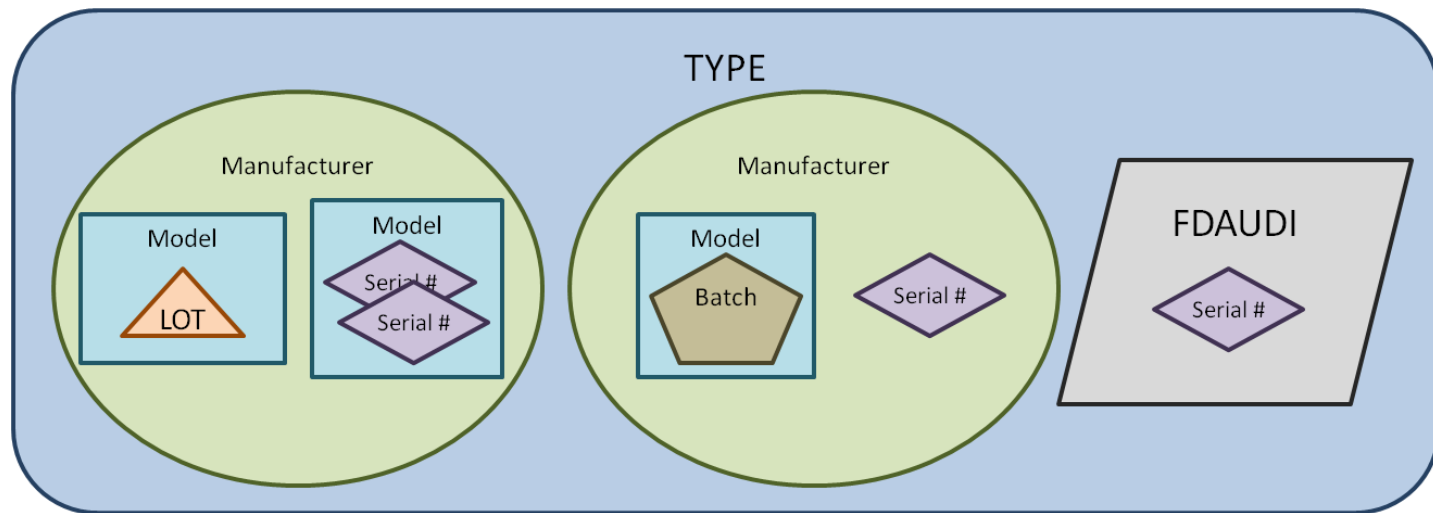

Graphic showing common relationships between identifier parameters for devices.

4.1.2 Examples for the Device Identifiers Domain Model

Example 1

This shows records for two devices where the sponsor felt that the type, manufacturer, model number, and serial number were necessary for unique identification. In addition, there was a post-marketing UDI identifier available for the first device.

- Rows 1-5 show the records for a device given a SPDEVID of ABC001
- Rows 5-8 show the records for a device given a SPDEVID of ABC999

Row	STUDYID	DOMAIN	SPDEVID	DISEQ	DIPARMCD	DIPARM	DIVAL
1	2011-001	DI	ABC001	1	TYPE	Device Type	MRI
2	2011-001	DI	ABC001	2	MANUF	Manufacturer	Acme Imaging
3	2011-001	DI	ABC001	3	MODEL	Model Number	45-JFI
4	2011-001	DI	ABC001	4	SERIAL	Serial Number	456789132-AXQ
5	2011-001	DI	ABC001	5	FDAUDI	FDA Unique Device Identifier	456789123xyz
6	2015-001	DI	ABC999	1	TYPE	Device Type	MRI
7	2015-001	DI	ABC999	2	MANUF	Manufacturer	Acme Imaging
8	2015-001	DI	ABC999	3	MODEL	Model Number	62-PLC
9	2015-001	DI	ABC999	4	SERIAL	Serial Number	215964564-NFS

Example 2

This example shows a case where a single device was used for all subjects at a given site. The device under study is an ESWT (extracorporeal shock wave treatment) for treatment of plantar fasciitis, and a single machine is used at each site. All devices in the study would be included in this table and therefore multiple devices are listed. Because SITEID is not a part of identifying each device, this table does not include SITEID and therefore does not record what device went to what site/device. The model and serial numbers are necessary to identify each device, and the device will be assigned to each subject via the Device-Subject Relationships domain (DR).

Row	STUDYID	DOMAIN	SPDEVID	DISEQ	DIPARMCD	DIPARM	DIVAL
1	ABCXYZ	DI	XYZ001	1	TYPE	Device Type	ESWT
2	ABCXYZ	DI	XYZ001	2	MODEL	Model	UR4000
3	ABCXYZ	DI	XYZ001	3	SERIAL	Serial Number	47821B
4	ABCXYZ	DI	QRS002	1	TYPE	Device Type	ESWT
5	ABCXYZ	DI	QRS002	2	MODEL	Model	UR4000
6	ABCXYZ	DI	QRS002	3	SERIAL	Serial Number	87232A

Example 3

This shows records for a device for which it was important to collect the type and manufacturer, but no more granular information was needed.

Row	STUDYID	DOMAIN	SPDEVID	DISEQ	DIPARMCD	DIPARM	DIVAL
1	2011-537	DI	ABC003	1	TYPE	Device Type	Cardiac Stent
2	2011-537	DI	ABC003	2	MANUF	Manufacturer	Stents, Ltd.

Example 4

This shows records for a study where two devices were used for treatment, one a thrombectomy device, which was identified using the type, model and serial number, and the other a stent, which was identified using only the type and a serial number.

Row	STUDYID	DOMAIN	SPDEVID	DISEQ	DIPARMCD	DIPARM	DIVAL
1	ABCXYZ	DI	XYZ001	1	TYPE	Device Type	Thrombectomy Device
2	ABCXYZ	DI	XYZ001	2	MODEL	Model	TR300
3	ABCXYZ	DI	XYZ001	3	SERIAL	Serial Number	452209BB
4	ABCXYZ	DI	QRS002	1	TYPE	Device Type	Coronary Stent
5	ABCXYZ	DI	QRS002	2	SERIAL	Serial Number	87232A

Example 5

This shows records for a device used in a study solely for obtaining measurements and the device is not under study. The only record required is a TYPE record.

Row	STUDYID	DOMAIN	SPDEVID	DISEQ	DIPARMCD	DIPARM	DIVAL
1	2011-537	DI	ABC003	1	TYPE	Device Type	MRI

4.2 DEVICE IN-USE - DU

du.xpt, Device In-Use - Findings, Version 1.0. One record per property or setting per time point per visit or test date per subject, Tabulation

Variable Name	Variable Label	Type	Controlled Terms, Codelist or Format	Role	Definition	Implementation Notes	Core
STUDYID	Study Identifier	Char		Identifier	Unique identifier for a study.	Unique identifier for a study.	Req
DOMAIN	Domain Abbreviation	Char	DU	Identifier	Two-character abbreviation for the domain.	Two-character abbreviation for the domain.	Req
USUBJID	Unique Subject Identifier	Char		Identifier	Identifier used to uniquely identify a subject across all studies for all applications or submissions involving the product.	Expected in this domain as devices may have settings or uses that either may not involve subjects (e.g., diagnostic tools) or devices that are removed from the study prior to contact with a subject (e.g., device has malfunction)	Exp
SPDEVID	Sponsor Device Identifier	Char		Identifier	Sponsor-defined identifier for the device.	It must be unique for each tracked unit of the device under study, and can be at whatever level of granularity the device should be identified (e.g., model or serial number, or combination of identifiers).	Exp
DUSEQ	Sequence Number	Num		Identifier	Sequence Number given to ensure uniqueness of device records within subject records within a domain.	May be any valid number. It should be unique within every subject/device combination.	Req
DUGRPID	Group ID	Char		Identifier	Identifier for a group or block of related records.	Used to tie together a block of related records in a single domain for a subject or a group of subject related records. Example: group records specifying all the settings for a specific imaging scan, such as field strength, repetition time and echo time.	Perm
DUREFID	Reference ID	Char		Identifier	Internal or external identifier.	This could be a scan code or equivalent.	Perm
DUSPID	Sponsor-Defined Identifier	Char		Identifier	Sponsor-defined reference number.	Perhaps pre-printed on the CRF as an explicit line identifier or defined in the sponsor's operational database.	Perm
DUTESTCD	Device In-Use Test Short Name	Char	(DUTESTCD)	Topic	Short name of the measurement, test, or examination described in DUTEST.	It can be used as a column name when converting a dataset from a vertical to a horizontal format. The value in DUTESTCD cannot be longer than 8 characters, nor can it start with a number (e.g. "1TEST"). DUTESTCD cannot contain characters other than letters, numbers, or underscores. Examples: COILSTR, CNTMEDIA.	Req
DUTEST	Device In-Use Test Name	Char	(DUTEST)	Synonym Qualifier	Verbatim name of the test or examination used to obtain the measurement or finding.	The value in DUTEST cannot be longer than 40 characters. Examples: Coil Strength, Contrast Media.	Req

CDISC Study Data Tabulation Model Implementation Guide for Medical Devices Version 1.0

Variable Name	Variable Label	Type	Controlled Terms, Codelist or Format	Role	Definition	Implementation Notes	Core
DUCAT	Category for Device In-Use	Char	*	Grouping Qualifier	Defines a category of related records.	For example, it can be used to define the type of device for which settings are recorded if DI is not used, for example, if the device is not under study. Alternatively, it could record the type of setting, e.g., HARDWARE vs. SOFTWARE	Perm
DUSCAT	Subcategory for Device In-Use	Char	*	Grouping Qualifier	A further categorization of a measurement or examination	For example, if DUCAT = SOFTWARE, DUSCAT might be NOMINAL or POST-ADJUSTMENT.	Perm
DUORRES	Result or Finding in Original Units	Char		Result Qualifier	Result of the measurement as originally received or collected.	DUORRES should contain the setting or other device condition in effect at the time the device was used.	Exp
DUORRESU	Original Units	Char	(UNIT)	Variable Qualifier	Original units in which the data were collected.	The unit for DUORRES. Examples: Tesla, mm.	Exp
DUSTRESC	Character Result/Finding in Std Format	Char		Result Qualifier	Contains the result value for all findings, copied or derived from DUORRES in a standard format or standard units.	DUSTRESC should store all results or findings in character format; if results are numeric, they should also be stored in numeric format in DUSTRESN. For example, if a test has results "NONE", "NEG", and "NEGATIVE" in DUORRES, and these results effectively have the same meaning, they could be represented in standard format in DUSTRESC as "NEGATIVE".	Exp
DUSTRESN	Numeric Result/Finding in Standard Units	Num		Result Qualifier	Used for continuous or numeric results or findings in standard format.	Is copied in numeric format from DUSTRESC. DUSTRESN should store all numeric test results or findings.	Exp
DUSTRESU	Standard Units	Char	(UNIT)	Variable Qualifier	Standardized unit used for DUSTRESC and DUSTRESN.	The unit for standardized results may or may not be the same as for the original results.	Exp
VISITNUM	Visit Number	Num		Timing	A clinical encounter number.	A Numeric version of VISIT, used for sorting.	Exp
VISIT	Visit Name	Char		Timing	Protocol-defined description of clinical encounter.	May be used in addition to VISITNUM and/or VISITDY.	Perm
VISITDY	Planned Study Day of Visit	Num		Timing	Planned study day of the visit based upon RFSTDTC in Demographics.	This value is usually derived.	Perm
DUDTC	Date/Time Device Used With Test/Setting	Char	ISO 8601	Timing	Date/time that the device was used with this setting	This is not the date/time that the setting was set on the device, but rather that date/time that a measurement or test was done using that setting.	Exp
DUDY	Study Day of Observation	Num		Timing	Study day of Device In-Use measurement, measured as integer days.	Algorithm for calculations must be relative to the sponsor-defined RFSTDTC variable in Demographics.	Perm

** Indicates variable may be subject to controlled terminology, (Parenthesis indicates CDISC/NCI code list code value)*

4.2.1 Assumptions for the Device In-Use Domain Model

1. DU Definition: The Device In-Use domain represents properties of the study device or ancillary device that are intentionally set when the device is used in the context of a study.
2. An ancillary device is a device used within a clinical trial to collect subject data / information (device or human subject), but that is not the target of the study (e.g., a MRI or CT machine whose settings must be recorded in a clinical trial studying heart failure, as required in the protocol). If settings for an ancillary device in a study need to be recorded and the device needs to be identified in the data, it is strongly recommended that DI be used for that identification. If a sponsor wishes to do it differently, they should discuss it with their regulatory reviewer.
3. Unlike Device Properties (DO – which describes device characteristics that do not change for the device during the trial), the DU domain captures characteristics and properties of a device that can vary from subject to subject or usage to usage over the course of a study. For example,
 - a. The full range of field strengths for a given MRI machine might be 0.5 to 3 Tesla, and these values would be captured in Device Properties. DU would record the specific settings used for a given subject, e.g., the field strength for the MRI scan for Subject 123 was 0.5 Tesla for visit 1.
 - b. The software for a pacemaker may start at version 1, and be updated to version 2 during the study. This change can be captured here. It would not go in DO as DO holds only characteristics that do not change during the study.
4. There are two primary identifiers in this domain: USUBJID and SPDEVID. Both are Expected. Either one or the other or both must be used. For example, a device under study will always have a SPDEVID, but may or may not have a USUBJID. An ancillary device (one not under study) for which In-Use data are required may have a USUBJID but may or may not have SPDEVID. In all cases where SPDEVID is used, it must be defined in the Device Identifiers (DI) domain.
5. There are cases where settings on devices used in studies might be reported in Device Exposure or Device In-Use, such as when the settings are changed to affect an efficacy response. Sponsors should confer with the appropriate regulatory authorities to determine where to submit this information
6. This domain is not intended to capture manufacturer-set (that is, nominal) settings, but rather the customized settings for a given usage.
7. Since any number of device settings (for example, coil strength, placement of leads) can be reported in this domain, each setting is represented by a separate row and is defined in the topic variable DUTESTCD. The original result goes into DUORRES.
8. DUREFID is the identifier for a unique scan or other test result to link a group of settings (for example, field strength or slice thickness in an MRI scan) to the results obtained from the reading or interpretation of the test (for example, the MRI image).
9. The DUSPID variable can be used to link this domain to other domains if necessary, such as AEs, Exposure and/or Device Events.
10. Note that in some of the examples below, variables that would be blank may have been dropped to conserve space. This does not mean that the variables cannot be used in the illustrated use case, merely that in this example they were not populated.
11. The following Qualifiers would not generally be used in DU: --MODIFY, --BODSYS, --POS,--ORNRLO, --ORNRHI, --STNRLO, --STNRHI, --STNRC, --NRIND, --RESCAT, --REASND, --XFN, --NAM, --LOINC, --SPEC, --SPCCND, --LOC, --METHOD, --FAST, --DRVFL, --EVAL, --TOX, --TOXGR, --SEV, --DTHREL, --LLOQ.

4.2.2 Examples for the Device In-Use Domain Model

Example 1:

This example shows data from one subject collected at two visits about parameters from an MRI imaging protocol. In this case, the image was used to obtain brain volume measurements, and the results of the image interpretation are reported in the Morphology domain. The parameters in DU can be linked to the measurement results using RELREC, and an illustration of this can be found in Section 5 Example 1. DUSPID is the same for each time point as the device settings were collected on a single record for each image taken.

Table 1, Rows 1-7: Represent 7 example Device In-Use records collected at the screening visit for a given subject.

Table 1, Rows 8-14: Represent 7 example Device In-Use records collected at the first treatment visit for the same subject.

Row	STUDYID	DOMAIN	USUBJID	SPDEVID	DUSEQ	DUGRPID	DUREFID	DUSPID	DUTESTCD	DUTEST	DUORRES
1	STUDYX	DU	2324-P0001	ABC174	1	DUMO1	222333-444555	1	COILSTR	Coil Strength	1.5
2	STUDYX	DU	2324-P0001	ABC174	2	DUMO1	222333-444555	1	ANTPLANE	Anatomical Plane	CORONAL
3	STUDYX	DU	2324-P0001	ABC174	3	DUMO1	222333-444555	1	STHICK	Slice Thickness	1
4	STUDYX	DU	2324-P0001	ABC174	4	DUMO1	222333-444555	1	MATRIX	Matrix	256X256
5	STUDYX	DU	2324-P0001	ABC174	5	DUMO1	222333-444555	1	SFTWRVER	Software Version	15.0
6	STUDYX	DU	2324-P0001	ABC174	6	DUMO1	222333-444555	1	FLDVIEW	Field of View	24
7	STUDYX	DU	2324-P0001	ABC174	7	DUMO1	222333-444555	1	RCBDWTH	Receiver Bandwidth	16
8	STUDYX	DU	2324-P0001	ABC174	8	DUMO2	444555-666777	2	COILSTR	Coil Strength	1.0
9	STUDYX	DU	2324-P0001	ABC174	9	DUMO2	444555-666777	2	ANTPLANE	Anatomical Plane	CORONAL
10	STUDYX	DU	2324-P0001	ABC174	10	DUMO2	444555-666777	2	STHICK	Slice Thickness	2
11	STUDYX	DU	2324-P0001	ABC174	11	DUMO2	444555-666777	2	MATRIX	Matrix	256X256
12	STUDYX	DU	2324-P0001	ABC174	12	DUMO2	444555-666777	2	SFTWRVER	Software Version	15.1
13	STUDYX	DU	2324-P0001	ABC174	13	DUMO2	444555-666777	2	FLDVIEW	Field of View	25
14	STUDYX	DU	2324-P0001	ABC174	14	DUMO2	444555-666777	2	RCBDWTH	Receiver Bandwidth	16

Row	DUORRESU	DUSTRESC	DUSTRESN	DUSTRESU	VISITNUM	VISIT	VISITDY	DUDTC	DUDY
1 (cont)	T	1.5	1.5	T	1	SCREENING	-7	2011-04-19	-7
2 (cont)		CORONAL			1	SCREENING	-7	2011-04-19	-7
3 (cont)	mm	1	1	mm	1	SCREENING	-7	2011-04-19	-7
4 (cont)		256X256			1	SCREENING	-7	2011-04-19	-7
5 (cont)		15.0	15.0		1	SCREENING	-7	2011-04-19	-7
6 (cont)	cm	24	24	cm	1	SCREENING	-7	2011-04-19	-7
7 (cont)	kHz	16	16	kHz	1	SCREENING	-7	2011-04-19	-7
8 (cont)	T	1.0	1.0	T	2	IMPLANTATION	1	2011-04-26	1
9 (cont)		CORONAL			2	IMPLANTATION	1	2011-04-26	1
10 (cont)	mm	2	2	mm	2	IMPLANTATION	1	2011-04-26	1
11 (cont)		256X256			2	IMPLANTATION	1	2011-04-26	1
12 (cont)		15.1	15.1		2	IMPLANTATION	1	2011-04-26	1
13 (cont)	cm	25	25	cm	2	IMPLANTATION	1	2011-04-26	1
14 (cont)	kHz	16	16	kHz	2	IMPLANTATION	1	2011-04-26	1

Example 2:

This example shows a software update applied to a pacemaker during the study.

Table 1, Row 1: Represents an example Device In-Use record collected at the screening visit that records the software version in use.

Table 1, Row 2: Represents an update to the software for the same device in the same subject from version 3.0 to version 3.02.

Row	STUDYID	DOMAIN	USUBJID	SPDEVID	DUSEQ	DUGRPID	DUREFID	DUTESTCD	DUTEST	DUORRES	DUORRESU
1	QL1059	DU	1059-001	BOEN37P	1	DUMO1	222333-444555	SFTWRVER	Software Version	3.0	
2	QL1059	DU	1059-001	BOEN37P	1	DUMO1	222333-444555	SFTWRVER	Software Version	3.02	

Row	DUSTRESC	DUSTRESN	DUSTRESU	VISITNUM	VISIT	VISITDY	DUDTC	DUDY
1 (cont)	3.0	3.0		1	SCREENING	-7	2011-04-19	-7
2 (cont)	3.02	3.02		5	VISIT 4	21	2011-05-16	21

4.3 DEVICE EXPOSURE - DX

dx.xpt, Device Exposure — Interventions, Version 1.0. One record per recorded intervention occurrence or constant treatment interval per subject, Tabulation

Variable Name	Variable Label	Data	Controlled Terms, Code list or Format	Role	Definition	Implementation Notes	Core
STUDYID	Study Identifier	Char		Identifier	Unique identifier for a study.	Unique identifier for a study.	Req
DOMAIN	Domain Abbreviation	Char	DX	Identifier	Two-character abbreviation for the domain.	Two-character abbreviation for the domain.	Req
USUBJID	Unique Subject Identifier	Char		Identifier	Identifier used to uniquely identify a subject across all studies for all applications or submissions involving the product.	Identifier used to identify a subject uniquely across all studies for all applications or submissions involving the product.	Req
SPDEVID	Sponsor Device Identifier	Char		Identifier	Sponsor-defined identifier for the device.	It must be unique for each tracked unit of the device under study, and can be at whatever level of granularity the device should be identified (e.g., model or serial number, or combination of identifiers).	Req
DXSEQ	Sequence Number	Num		Identifier	Sequence Number given to ensure uniqueness of device records within subject records within a domain.	May be any valid number. It should be unique within every subject/device combination.	Req
DXGRPID	Group ID	Char		Identifier	Identifier that ties together a block of related records in a single domain for a subject.	For example, if a device is inserted that delivers radiation, DXGRPID could be used to tie the records for the device and the radiation together for each course of therapy.	Perm
DXSPID	Sponsor-Defined Identifier	Char		Identifier	Sponsor-defined reference number.	Examples: a number pre-printed on the CRF as an explicit line identifier or record identifier defined in the sponsor's operational database.	Perm
DXTRT	Name of Device Exposure or Output	Char		Topic	Name of the device or the exposure outputs that are delivered or administered via the device. This should match the definitions as described in the trial summary domain and/or the protocol.	Example: coronary stent, extracorporeal shock wave treatment, hyaluronic acid	Req
DXCAT	Category for Device Exposure	Char	*	Grouping Qualifier	Used to define a category of device exposures	For example, for a subject who had radiation delivered through an implanted catheter, DXCAT could be used to group the radiation records vs. the catheter records.	Perm
DXSCAT	Subcategory for Device Exposure	Char	*	Grouping Qualifier	A further categorization of device exposures	If DXCAT captures the radiation vs. catheter records (see DXCAT), then DXSCAT might capture the type of catheter if more than one was used.	Perm

CDISC Study Data Tabulation Model Implementation Guide for Medical Devices Version 1.0

Variable Name	Variable Label	Data	Controlled Terms, Code list or Format	Role	Definition	Implementation Notes	Core
DXDOSE	Exposure per Administration	Num		Record Qualifier	Amount of DXTRT administered/delivered per administration.	Dose if captured as a numeric value. Dose should only appear once in DXDOSE, DXDOSTXT or DXDOSTOT	Perm
DXDOSTXT	Device Exposure Description	Char		Record Qualifier	Exposure amounts or a range of exposure information collected in text form.	Units may be stored in DXDOSU. Example: 200-400, 15-20. Dose should only appear once in DXDOSE, DXDOSTXT or DXDOSTOT	Perm
DXDOSU	Device Exposure Units	Char	(UNIT)	Variable Qualifier	Units for DXDOSE, DXDOSTXT, and DXDOSTOT.	Examples: pulses, ml	Perm
DXDOSFRQ	Device Exposure Frequency per Interval	Char	(FREQ)	Variable Qualifier	Exposure frequency per interval.	Usually expressed as the number of repeated administrations of DXDOSE within a specific time period. Examples: CONTINUOUS, PRN, Q2M (Every 2 months)	Perm
DXDOSTOT	Total Daily Device Exposure	Num		Record Qualifier	Total daily exposure of DXTRT using the units in DXDOSU	. Total exposure over a period other than day could be recorded in a separate Supplemental Qualifier variable.	Perm
DXDOSRGM	Intended Device Exposure Regimen	Char		Variable Qualifier	Text description of the (intended) schedule or regimen for the Intervention.	Examples: TWO WEEKS ON, TWO WEEKS OFF.	Perm
DXROUTE	Route of Administration	Char	(ROUTE)	Variable Qualifier	Route of administration for DXTRT.	Examples: EXTRACORPOREAL, INTRA-ARTICULAR, HEMODIALYSIS	Perm
DXLOC	Location of Device Exposure	Char		Record Qualifier	Anatomic location of exposure	Examples: Left knee, OD	Perm
DXLAT	Laterality of Device Exposure	Char		Variable Qualifier	Qualifier for anatomical location further detailing laterality	Examples: Right, Left, Bilateral	
DXMETHOD	Method of Device Exposure	Char	*	Record Qualifier	Method of device exposure.	Example: Implantation, Injection	Perm
DXADJ	Reason for Exposure Adjustment	Char		Record Qualifier	Describes reason why the exposure was adjusted from protocol-specified or expected exposure levels.	Example: PAIN	Perm
DXSTDTC	Start Date/Time of Device Exposure	Char	ISO 8601	Timing	Start date and time of exposure	As defined by the sponsor	Exp
DXENDTC	End Date/Time of Device Exposure	Char	ISO 8601	Timing	End date and time of exposure.	As defined by the sponsor	Perm
DXSTDY	Study Day of Start of Device Exposure	Num		Timing	Study day of start of exposure.	Study day of start of exposure relative to the sponsor-defined RFSTDTC.	Perm

Variable Name	Variable Label	Data	Controlled Terms, Code list or Format	Role	Definition	Implementation Notes	Core
DXENDY	Study Day of End of Device Exposure	Num		Timing	Study day of end of exposure	Study day of end of exposure relative to the sponsor-defined RFSTDTC.	Perm
DXDUR	Duration of Device Exposure	Char	ISO 8601	Timing	Collected duration for a treatment episode.	Used only if collected on the CRF and not derived from start and end date/times.	Perm

* Indicates variable may be subject to controlled terminology, (Parenthesis indicates CDISC/NCI code list code value)

4.3.1 Assumptions for the Device Exposure Domain Model

1. DX Definition: The Device Exposure domain records the details of a subject’s direct interaction or contact with a medical device or the output from a medical device, usually but not always the device under study. This device may be used by the subject, on the subject, or implanted into the subject. Examples include but are not limited to stents, drug delivery systems, and any other item under study that is defined as a device in the applicable regulations.
2. The DX data may be captured on a CRF, downloaded from a device, or derived. The sponsor determines the appropriate method.
3. The structure of the DX domain is one record per exposure intervention episode or constant-exposure interval per subject. It is the sponsor's responsibility to define an intervention episode. This definition may vary based on the sponsor's requirements for review and analysis. The submission dataset structure may differ from the structure used for collection. One common approach is to submit a new record when there is a change in the exposure regimen. Another approach is to collapse all records for an exposure to a summary level with exposure range. Other approaches may also be reasonable as long as they meet the sponsor's evaluation requirements.
4. A DX domain is expected whenever there is individual subject exposure to a device under study. Device studies in which only pooled samples are used, for example, some diagnostic devices, may not require a DX domain. In these cases, a subject’s sample is part of a pooled sample, and the subject is never in contact with the device, therefore there is no exposure to report. Note that contact can be directly between subject and device, or between subject and a device output.
5. In cases where a device/drug combination is being studied, the device exposure data would generally be submitted in DX and the drug exposure data would generally be submitted in EX, but each sponsor should confer with the appropriate regulatory authorities to determine the right datasets.
6. There are cases where settings on devices used in studies might be reported in Device Exposure or Device In-Use, such as when the settings are changed to affect an efficacy response. Sponsors should confer with the appropriate regulatory authorities to determine where to submit this information.
7. Categorization and Grouping
 - a. DXCAT and DXSCAT may be used when appropriate to categorize treatments into categories and subcategories. For example, if a study uses several different devices, DXCAT may be set to “ACTIVE COMPARATOR.” Such categorization may not be useful in most studies, so these variables are permissible and not expected.
8. Device Exposure Treatment Description
 - a. DXTRT captures the name of the investigational medical device and is the topic variable. It is a required variable and must have a value. DXTRT should avoid unnecessarily repeating characteristics found in the Device Properties (DO) domain.
9. Timing Variables

- a. The timing of exposure to the study device is captured by the start/end date and start/end time of each intervention episode or constant exposure interval, as defined by the sponsor.
- 10. Additional Interventions Qualifiers
 - a. Other additional Qualifiers from the SDTM Interventions Class may be added to this domain.
- 11. Note that in some of the examples below, variables that would be blank may have been dropped to conserve space. This does not mean that the variables cannot be used in the illustrated use case, merely that in this example they were not populated.
- 12. The DXSPID variable can be used to link this domain to other domains if necessary, such as AEs, Exposure and/or Device Events.

4.3.2 Examples for the Device Exposure Domain Model

Example 1: Injection of hyaluronic acid (HA) into knee for treatment of osteoarthritis

In this example, the study is investigating the safety and efficacy of the device ‘Hyaluronic Acid’ given into the intra-articular space of the knee joint to relieve the pain associated with osteoarthritis through lubrication. The product is administered once a week for three weeks. Hyaluronic acid provides physical lubrication in the joint, and is considered to be a device by the manufacturer and the regulators, even though it has many of the characteristics of a drug.

Row	STUDYID	DOMAIN	USUBJID	SPDEVID	DXSEQ	DXSPID	DXTRT	DXDOSE	DXDOSU
1	ABCXYZ	DX	001-001	LOTABC	1	1	HYALURONIC ACID	2	mL
2	ABCXYZ	DX	001-001	LOTABC	2	2	HYALURONIC ACID	2	mL
3	ABCXYZ	DX	001-001	LOTXYZ	1	3	HYALURONIC ACID	2	mL

Row	DXDOSFRQ	DXDOSRGM	DXROUTE	DXLOC	DXSTDTC	DXENDTC	DXSTDY	DXENDY	DXDUR
1 (cont)	ONCE	1X/WK FOR 3 WEEKS	INTRA-ARTICULAR	LEFT KNEE	2010-05-02T12:15	2010-05-02T12:17	1	1	
2 (cont)	ONCE	1X/WK FOR 3 WEEKS	INTRA-ARTICULAR	LEFT KNEE	2010-05-09T13:15	2010-05-09T13:17	8	8	
3 (cont)	ONCE	1X/WK FOR 3 WEEKS	INTRA-ARTICULAR	LEFT KNEE	2010-05-13T13:15	2010-05-13T13:17	12	12	

Example 2: ESWT (extracorporeal shock wave treatment) for treatment of plantar fasciitis

In this example a device that delivers shock wave pulses is used to treat plantar fasciitis (inflammation of the plantar fascia in the heel). The study is investigating the safety and efficacy of this single device treatment that has is used in two orientations within the heel receiving pulses (in-line, and 45 deg medial to plantar). The orientation information is captured in Device in Use (DU). This example shows a patient that had an aborted treatment due to an adverse event.

Row	STUDYID	DOMAIN	USUBJID	SPDEVID	DXSEQ	DXSPID	DXTRT	DXDOSE	DXDOSTXT	DXDOSFRQ	DXDOSTOT	DXDOSU
1	ABCXYZ	DX	001-001	SERAZZ3	1	1	EXTRACORPOREAL SHOCK WAVE TREATMENT	500		ONCE		PULSES
2	ABCXYZ	DX	001-001	SERAZZ3	2	2	EXTRACORPOREAL SHOCK WAVE TREATMENT	400		ONCE		PULSES

Row	DXDOSRGM	DXROUTE	DXLOC	DXADJ	DXSTDTC	DXENDTC	DXSTDY	DXENDY	DXDUR
1 (cont)	500 pulses/treatment session	Extracorporeal	Right Plantar Fascia		2010-05-02T12:15	2010-05-02T12:30	1	1	
2 (cont)	500 pulses/treatment session	Extracorporeal	Right Plantar Fascia	Adverse Event	2010-05-03T14:31	2010-05-03T14:45	2	2	

Example 3: APBI (Accelerated partial breast irradiation) with radiation delivery device

This study is investigating the functional delivery of the radiation treatment to the breast via a balloon catheter system. The system is inserted into a tumor cavity post excision. After surgery the catheter is left inside the cavity for 5 days. During the time of implant the radiation is delivered from a HDR device (“seed”) through the part of the catheter system remaining outside the body twice per day in two separate fractions. In this example there is a recording of the surgical placement of the catheter system, and the first 4 fraction records. The location of the placement and radiation delivery is coded. In this example, the radiation information is submitted in DX, but there may be cases where it would more appropriately be recorded in Device In-Use (DU).

Row	STUDYID	DOMAIN	USUBJID	SPDEVID	DXSEQ	DXSPID	DXGRPID	DXTRT	DXDOSE	DXDOSFRQ	DXDOSU
1	ABCXYZ	DX	001-001	SER56XA	1	1	CATH	ABC balloon catheter system		ONCE	
2	ABCXYZ	DX	001-001	SER44531	1	2	RAD	APBI	3.4	BID	Gy
3	ABCXYZ	DX	001-001	SER44531	2	3	RAD	APBI	3.4	BID	Gy
4	ABCXYZ	DX	001-001	SER44531	3	4	RAD	APBI	3.4	BID	Gy
5	ABCXYZ	DX	001-001	SER44531	4	5	RAD	APBI	3.4	BID	Gy

Row	DXDOSTOT	DXDOSRGM	DXROUTE	DXLOC	DXSTDTC	DXENDTC	DXSTDY	DXENDY	DXDUR
1 (cont)		ONCE	Intradermal	LUO*	2010-05-02T12:15	2010-05-010T13:30	1	9	
2 (cont)		5 DAYS	Intradermal	LUO	2010-05-03T08:31	2010-05-03T08:45	2	2	
3 (cont)		5 DAYS	Intradermal	LUO	2010-05-03T15:31	2010-05-03T15:45	2	3	
4 (cont)		5 DAYS	Intradermal	LUO	2010-05-04T08:31	2010-05-04T08:45	3	3	
5 (cont)		5 DAYS	Intradermal	LUO	2010-05-04T15:31	2010-05-04T15:45	3	3	

* Left Upper Outer Breast.

Example 4: Implanted Cervical Disc

This is an example of a study investigating the safety and efficacy of a cervical disc replacement. In this example there are two separate patients, one who had the device implanted and evaluated throughout the study (001-001), and the second (002-001) who had the device explanted on Day 7.

Row	STUDYID	DOMAIN	USUBJID	SPDEVID	DXSEQ	DXSPID	DXTRT	DXDOSE	DXDOSTXT	DXDOSU	DXDOSFRQ
1	ABCXYZ	DX	001-001	SER45001	1	1	Artificial Cervical Disc	1		UNIT	ONCE
2	ABCXYZ	DX	002-001	SER86002	1	1	Artificial Cervical Disc	1		UNIT	ONCE

Row	DXMETHOD	DXLOC	DXSTDTC	DXENDTC	DXSTDY	DXENDY	DXENRTPT	DXENTPT
1 (cont)	SURGICAL	C3-4	2010-05-02T12:15		1		ONGOING	CLOSEOUT
2 (cont)	SURGICAL	C3-4	2010-05-02T13:15	2010-05-09T13:17	1	8		

Example 5: Suture Material

This is an example of a study investigating the safety and efficacy of a particular suture material in closing wounds. In this example, the same subject had two wounds. One was on the left forearm and was sutured using the material under study, while the other was on the right thigh and was sutured using a control.

Row	STUDYID	DOMAIN	USUBJID	SPDEVID	DXSEQ	DXTRT	DXDOSE	DXDOSTXT	DXDOSU
1	P47-923	DX	923-021	STRONG2	1	Strong Suture No 2	15		cm
2	P47-923	DX	923-021	COMP465	1	GenSuture	12		cm

Row	DXMETHOD	DXLOC	DXLAT	DXSTDTC	DXENDTC	DXSTDY	DXENDY
1 (cont)	SURGICAL	FOREARM	LEFT	2011-12-24T15:25	2001-12-30T09:38	1	7
2 (cont)	SURGICAL	THIGH	RIGHT	2011-12-24T15:45	2001-12-30T09:32	1	7

4.4 DEVICE EVENTS - DE

de.xpt, Device Events - Events, Version 1.0. One record per event per device, Tabulation

Variable Name	Variable Label	Data type	Controlled Terms, Code list or Format	Role	Definition	Implementation Notes	Core
STUDYID	Study Identifier	Char		Identifier	Unique identifier for a study.	Unique identifier for a study.	Req
DOMAIN	Domain Abbreviation	Char	DE	Identifier	Two-character abbreviation for the domain.	Two-character abbreviation for the domain.	Req
USUBJID	Unique Subject Identifier	Char		Identifier	Identifier used to uniquely identify a subject across all studies for all applications or submissions involving the product.	Expected rather than required because events may happen to or with a device that do not involved subjects, and may even be before the device was in contact with a subject. In these cases there may not be a value for USUBJID.	Exp
SPDEVID	Sponsor Device Identifier	Char		Identifier	Sponsor-defined identifier for the device.	It must be unique for each tracked unit of the device under study, and can be at whatever level of granularity the device should be identified (e.g., model or serial number, or combination of identifiers).	Req
DESEQ	Device Events Sequence Number	Num		Identifier	Sequence Number given to ensure uniqueness of device records within subject records within a domain.	May be any valid number. It should be unique within every subject/device combination. If there is no USUBJID associated with the event, DESEQ should be unique within each SPDEVID.	Req
DESPID	Sponsor-Defined Identifier	Char		Identifier	Sponsor-defined reference number.	Perhaps pre-printed on the CRF as an explicit line identifier or defined in the sponsor's operational database. Note that it does not have to be numeric.	Perm
DETERM	Reported Term for Device Event	Char		Topic	Verbatim name of the observed event.	Examples: Screw Breakage, Fissure Formation, Battery Issue	Req
DEMODYFY	Modified Device Event Name	Char		Synonym Qualifier	The modified text for DETERM	If DETERM is modified, then the modified text is placed here.	Perm
DEDECOD	Device Events Dictionary-Derived Term	Char	* FDA's Device Problem Codes	Synonym Qualifier	Dictionary-derived form of the event described in DETERM.	Dictionary-derived text description of DETERM or DEMODYFY. The name and version of the dictionary used to map terms must be provided in a Define.XML ExternalCodeList element.	Req
DECAT	Category of Device Event	Char	*	Grouping Qualifier	Used to define a categorization level for events.	For example, MALFUNCTION vs. CALIBRATION	Perm
DESCAT	Subcategory of Device Event	Char	*	Grouping Qualifier	Used to define a further category level for events.	For example, EXTERNAL vs. INTERNAL	Perm
DEPRESP	Pre-Specified Device Event	Char	(NY)	Record Qualifier	Used to indicate whether (Y/null) information about a specific event was solicited on the CRF.	For example, DETERM could contain a list of malfunctions that are being specifically evaluated. DEPRESP would identify those (Y), while any spontaneous events would have DEPREST = null.	Perm
DEOCCUR	Device Event	Char	(NY)	Record	When information about specific events is	Values are null for events not specifically solicited.	Perm

CDISC Study Data Tabulation Model Implementation Guide for Medical Devices Version 1.0

Variable Name	Variable Label	Data type	Controlled Terms, Code list or Format	Role	Definition	Implementation Notes	Core
	Occurrence			Qualifier	solicited, DEOCCUR is used to indicate whether or not (Y/N) a particular pre-specified event occurred.		
DESTAT	Device Event Collection Status	Char	(ND)	Record Qualifier	The status indicates that the pre-specified question was not answered.	For example, if equipment operation requires checking, such as checking an event log to detect events. Capturing that the checks were not completed may be relevant to interpreting the study data.	Perm
DEREASND	Reason Device Event Not Collected	Char			Reason DESTAT was “not done”	This variable should only be used if there are prespecified events.	Perm
DESEV	Device Event Severity	Char	*		Severity of Event	Terms Describing Severity of Event (e.g., the severity of a Malfunction)	Perm
DEACNDEV	Action Taken with Device	Char	*		Describes Action Taken with respect to the device	Action Taken may include removal, calibration, reprogramming, etc. Action is usually in response to some event, for example, a subject’s adverse event	Perm
VISITNUM	Visit Number	Num		Timing	Clinical encounter number.	Numeric version of VISIT, used for sorting.	Exp
VISIT	Visit Name	Char		Timing	Protocol-defined description of clinical encounter.	May be used in addition to VISITNUM and/or VISITDY.	Perm
VISITDY	Planned Study Day of Visit	Num		Timing	Planned study day of the visit based upon RFSTDTC in Demographics.	This value is usually derived.	Perm
DEDTC	Date of Device Event Data Collection	Char	ISO 8601	Timing	Date the device event information was collected.	This may be reported if the event (e.g., malfunction) is discovered on a different date from the event	Perm
DESTDTC	Start Date/Time of Device Event	Char	ISO 8601	Timing	Start date/time of the device event.	If the event happened at a single point in time, DESTDTC is used.	Perm
DEENDTC	End Date/Time of Device Event	Char	ISO 8601	Timing	End date/time of the device event.	If an event lasted over a period of time, DEENDTC can be used to capture the end date/time.	Perm
DEDY	Study Day of Device Event Data Collection	Num		Timing	Study day of Device Event observation, measured as integer days.	Algorithm for calculations must be relative to the sponsor-defined RFSTDTC variable in Demographics.	Perm
DESTDY	Study Day of Device Event Start Date/Time	Num		Timing	Study day of start of Device Event, measured as integer days.	Algorithm for calculations must be relative to the sponsor-defined RFSTDTC variable in Demographics.	Perm
DEENDY	Study Day of Device Event End Date/Time	Num		Timing	Study day of end of Device Event, measured as integer days.	Algorithm for calculations must be relative to the sponsor-defined RFENDTC variable in Demographics.	Perm

* Indicates variable may be subject to controlled terminology; sponsor will identify the controlled terminology in define.XML.

4.4.1 Assumptions for the Device Events Domain Model

1. Device Events Definition: The Device Events domain captures information about a variety of activities that can occur to or with the device, for example, malfunctions, calibrations, or parts replacement. It is an optional domain, to be used only if the sponsor has events that should be reported. Records are specific to an individual device. The entries may be related to one or many subjects and visits, depending upon the type of device and scope of its use.
2. USUBJID is Expected in this domain. See CDISC Notes for further explanation.
3. In some cases, a device event may occur but have no effect on a study, for example, a malfunction occurring if a device is damaged in transit or setup before its use in a study. It is assumed that these events will be reported elsewhere.
4. Depending upon the type of device, an event such as a malfunction may impact one subject (e.g., implantable, disposable, single-use devices) or many subjects, visits, and findings (e.g., diagnostic, imaging devices). This could require multiple records, one for each event for each associated subject (USUBJID) or device, as appropriate. In this case, a single DEREVID value would identify multiple records representing the subject-by-subject impact of the malfunction.
5. There are two broad cases in which device events (e.g., malfunctions) may be recorded: 1) the device is under study, or 2) the device is ancillary, that is, used simply to obtain a finding, but some properties of the device are recorded within the study.
6. If there is a malfunction, device exposure (DX) and device in-use settings (DU) may also be recorded. In some cases, it is possible that only the most general definition of the device (e.g., x-ray, CT, ultrasound) may be identified.
7. If a malfunction or other event results in an adverse event, then that information should be recorded in the Adverse Events (AE) domain (see SDTMIG, AE domain). The relationship between the AE and the Device Events can be recorded on the CRF using DESPID and/or DEAEENO. DEAEENO would be a data capture (CDASH) variable that is not submitted in SDTM-based datasets, but is used to create a RELREC that links the event records.
8. The present revision of DE assumes that a device event such as a malfunction is associated with one or more subjects and visits, and at most one AE per subject. More complex cases are deferred to future revisions.
9. DEENDTC can be used, for example, if a malfunction occurs during a deployment and it is repaired.
10. If this domain is used to capture device malfunctions, and the FDA's Device Problem Code controlled terminology list is used (available at <http://www.fda.gov/MedicalDevices/Safety/ReportaProblem/EventProblemCodes/ucm134845.htm>), then any codes beyond the Preferred Term can be included as Supplemental Qualifiers. See SDTMIG Appendix C5 for information about including hierarchies of terms.
11. Note that in some of the examples below, variables that would be blank may have been dropped to conserve space. This does not mean that the variables cannot be used in the illustrated use case, merely that in this example they were not populated.
12. The following Qualifiers would not generally be used in DE: --BODSYS, --SER,--ACN, --REL, --RELNST, --PATT, --OUT, --SCAN, --SCONG, --SDISAB, --SDTH, --SHOSP, --SLIFE, --SOD, --SMIE, --CONTRT, --TOX, -TOXGR.

4.4.2 Examples for the Device Events Domain Model

Example 1: Malfunction Events: In this example, two units of the device have suffered a series of failures. Each failure is recorded separately.

Row	STUDYID	DOMAIN	USUBJID	SPDEVID	DESEQ	DETERM	DEDECOD	DECAT	DESEV	DEDTC	DESTDTC
1	ABCXYZ	DE	1001	1001001	1	Minor screw breakage	Screw breakage	Equipment Failure	Minor	2009-11-02	2009-11-01
2	ABCXYZ	DE	1001	1001001	2	Shallow fissure formation	Fissure	Equipment Failure	Minor	2009-12-15	2009-12-13
3	ABCXYZ	DE	1002	999981	1	Battery will not charge	Battery charge failure	Equipment Failure	Major	2009-10-13	2009-10-10
4	ABCXYZ	DE	1002	999981	2	Firmware Consistency Fail 103	Firmware failure 103	Software Malfunction	Major	2010-01-03	2010-01-03

Example 2:

Row 1: This example shows a malfunction of an MRI calibration affecting one subject. In this case the individual MRI unit is not under study (e.g., when the MRI is used to obtain study measurements), and the sponsor decided to use the site number in SPDEVID.

Row 2: The second record is a malfunction of the device under study where all subjects for the day were affected. If this single record is sufficient detail for the sponsor’s requirements then no further records would be added, but if there were a need to associate the malfunction with each subject (e.g., it led to several AEs) then a record could be added for each affected subject. USUBJID is null because this device malfunction was not specific to one subject.

Row 3: The third record shows a malfunction for a specific device under study and the associated subject.

Row	STUDYID	DOMAIN	USUBJID	SPDEVID	DESEQ	DETERM	DEDECOD	DECAT	DESEV	DEDTC	DESTDTC
1	ABC-123	DE	2022	Site 22	1	First calibration failed	Calibration failed	Calibration Failure	Minor	2010-01-01	2009-12-28
2	ABC-456	DE		15033	1	Data Loss	Data failure	Data Storage Failure	Major	2009-01-06	2009-01-05
3	ABC-789	DE	2222	334-XRS-09	1	Alignment Failure	Calibration failed	Calibration Failure	Major	2009-01-05	2009-01-05

Example 3: This example shows how failures for implanted devices could be modeled.

Row	STUDYID	DOMAIN	USUBJID	SPDEVID	DESEQ	DETERM	DEDECOD	DECAT	DESEV	DEDTC	DESTDTC
1	ABCXYZ	DE	2022	X1010785	1	Calibration Failed	Calibration failed	Equipment Failure	Medium	2010-01-01	2009-12-28
2	ABCXYZ	DE	2133	15033	1	Internal communication failure	Communications failure	Equipment Failure	Medium	2009-01-05	2009-01-05
3	ABCXYZ	DE	2133	334-XRS-09	2	Internal communication failure	Communications failure	Equipment Failure	Medium	2009-01-05	2009-01-05

Example 4:

Row 1: This example shows a maintenance and calibration checks associated with a QA schedule of an MRI calibration where all subjects after the event were affected. The DEDTC variable captures when the information was recorded and/or discovered. DESTDTC records when the event happened. In this case, a software update occurred, and a maintenance event recorded some issue, which was only found subsequently on the 6th. This allows sponsors to determine if anything of importance happened during that interval, e.g., if any subjects were exposed to the device. If this single record is sufficient detail for the sponsor’s requirements then no further records would be added, but if there were a need to associate the QA event with each subject (e.g., if the information collected during the maintenance event were needed to calibrate results for subsequent cases) then a record could be added for each affected subject.

Row 2: The second record shows a software version update for a specific device under study. USUBJID is null because the software update applies to all subjects.

Row	STUDYID	DOMAIN	SPDEVID	USUBJID	DESEQ	DETERM	DEDECOD	DECAT	DESEV	DEDTC	DESTDTC
1	ABC-456	DE	15033		1	Routine device diagnostics performed	Scheduled Maintenance	Scheduled Maintenance	Minor	2009-01-06	2009-01-05
2	ABC-789	DE	15033		2	Control software updated	Software Update	Software Update	Major	2009-01-05	2009-01-05

4.5 DEVICE TRACKING AND DISPOSITION - DT

dt.xpt, Device Tracking and Disposition - Events, Version 1.0 One record per device tracking event, Tabulation

Variable Name	Variable Label	Type	Controlled Terms, Code list or Format	Role	Definition	Implementation Notes	Core
STUDYID	Study Identifier	Char		Identifier	Unique identifier for a study.	Unique identifier for a study.	Req
DOMAIN	Domain Abbreviation	Char	DT	Identifier	Two-character abbreviation for the domain.	Two-character abbreviation for the domain.	Req
SPDEVID	Sponsor Device Identifier	Char		Identifier	Sponsor-defined identifier for the device.	It must be unique for each tracked unit of the device under study, and can be at whatever level of granularity the device should be identified (e.g., model or serial number, or combination of identifiers).	Req
DTSEQ	Sequence Number	Num		Identifier	Sequence Number given to ensure uniqueness of device records within subject records (if applicable) within a domain.	May be any valid number. Should be unique within each SPDEVID.	Req
DTTERM	Reported Term for the Tracking Event	Char	*	Topic	Verbatim or preprinted term for the activity that occurs.	Example: Shipped, Returned, Installed, Implanted, Explanted	Req
DTMODIFY	Modified Reported Term	Char		Synonym Qualifier	Modified term entered to allow mapping of verbatim term to dictionary term	If DTTERM is modified to facilitate coding, then DTMODIFY will contain the modified text.	Perm
DTDECOD	Standardized Tracking Term	Char	*	Synonym Qualifier	Dictionary-derived text description of DTTERM or DTMODIFY.	If an external controlled terminology is used, the name and version of the dictionary used to map terms must be provided in a Define.XML ExternalCodeList element.	Perm
DTPARTY	Party Responsible for the Device	Char	*	Record Qualifier	Person or organization accountable for the device at the conclusion of the action specified in DTTERM.	Describes the person or organization that is accountable for the device defined in DTTERM. For example: if DTTERM = SHIPPED, DTPARTY would contain the transfer recipient, e.g., SITE. If DTTERM = IMPLANTED then DTPARTY would contain SUBJECT.	Req

Variable Name	Variable Label	Type	Controlled Terms, Code list or Format	Role	Definition	Implementation Notes	Core
DTPRTYID	Responsible Party Identifier	Char		Variable Qualifier	An identifier for the responsible group/role (e.g. site, subject).	The value of the responsible party identified in DTPARTY. For example, if DTPARTY is SUBJECT, DTPRTYID would contain the subject number.	Exp
DTCAT	Category for Device Tracking Event	Char	*	Grouping Qualifier	Define a categorization level for a group of related records.	Examples: categorize by tracking event type, for example, DOMESTIC vs. INTERNATIONAL	Exp
DTSCAT	Subcategory for Device Tracking Event	Char		Grouping Qualifier	Defines a further categorization level for a group of related conditions or events.	A further categorization of the event.	Perm
DTDTC	Date/Time of Device Tracking Event Collection	Char	ISO 8601	Timing	Date/Time of the tracking event information was collected.	Will generally be the same as the date the tracking event started, but it can differ.	Perm
DTSTDTC	Start Date/Time of Device Tracking Event	Char	ISO 8601	Timing	Start date/time of tracking event.	A tracking event (e.g., SHIPPED, RECEIVED) is usually a point in time, which is why only the start date/time is included. If an event occurs over a longer period, the stop date/time may be included from the SDTM model.	Req

* Indicates variable may be subject to controlled terminology; sponsor will identify the controlled terminology in *define.XML*.

4.5.1 Assumptions for the Device Tracking and Disposition Domain Model

1. DT Definition: The Device Tracking and Disposition domain represents tracking events for a given device. This could include initial shipment, deployment, return, destruction, loss, etc. Different tracking events would be relevant to different types of devices. For example, an MRI machine might be shipped to a hospital and remain there, while an implantable stent might be shipped to a site and then shipped back to the sponsor if found to be defective.
2. Only tracking events that are the sponsor’s responsibility are captured in this domain. If that responsibility is formally passed to another entity, such as hospital staff tracking an MRI machine within their facility, then tracking data will not generally appear in DT. This is governed by local regulations and sponsor/site practices.
3. This domain is intended to demonstrate “device accountability,” and can be submitted in two ways. Tracking data can be captured and submitted that indicate each party who is accountable for the device from the time it leaves the sponsor facility to its final state such that the dataset accounts for the device at all times. The last record would effectively be the final disposition of the device. Alternatively, a single disposition record for each device could be submitted, representing the status of each device at the time of submission and the individual

- tracking event information remains at the site and sponsor locations and is available for inspection. This flexibility allows sponsors to track devices either at every move or only report a final disposition at study end.
4. This domain is not intended to report details about the deployment of a device to a subject except insofar as the device is physically with the subject (for example, implantation of a stent). Subject-specific deployment information would usually more appropriately be captured in the Device Exposure domain. In some cases this may result in some duplication of data between DX and DT, but the data are intended for very different purposes and will often capture different details.
 5. The level of granularity of the device identification in this domain will vary by device type and sponsor practice, and is defined in Device Identifiers. In cases where a group of devices is tracked together, such as a box of orthopedic screws, a given SPDEVID may represent multiple individual units that are not individually tracked and may be split and shipped to different sites. Capture of this information may require the use of the Findings About domain (see SDTMIG Section 6.4).
 6. In cases where a device is comprised of a number of components (e.g., a pacemaker with leads and software), the sponsor may choose to track the overall device using its SPDEVID or track the identifiers for the individual components, or both, whatever is more appropriate. Subsequent versions of this document will address the details of tracking components and of associating them with a device.
 7. If this domain is populated, there should be at least 1 record in this domain for every tracked unit of the device under study associated with a study that leaves the sponsor's facility or manufacturing location. There may be multiple records per device.
 8. DTPARTY and DTPRTYID together identify the individual or organization that takes responsibility for the device as a result of the action in DTTERM. For example, if DTTERM is SHIPPED, DTPARTY would be a general term defining the type of responsible party, such as SITE, and DTPRTYID would contain the site identifier, such as 02.
 9. Usually DTPARTY and DTPRTYID refer to who has possession of the device after the action in DTTERM. In the cases where a device is lost, destroyed or removed, for example, DTPARTY and DTPRTYID may be null.
 10. Tracking events do not have start and end dates since they do not span an interval (e.g. shipped date) but occur at a single date/time (e.g., implantation date).
 11. Relative study days (--DY) are not included in this domain as there may be no association with a subject, and relative days are calculated in comparison to a subject's reference start date. If sponsors need to include this information, they may include --DY but its derivation must follow the rules in the SDTMIG.
 12. The data in this domain may come from a variety of sources, such as a CRF, a shipping log or a transfer document (such as when devices are issued as supplies or samples for engineers to take to sites), and may be partly or wholly derived.
 13. Note that in some of the examples below, variables that would be blank may have been dropped to conserve space. This does not mean that the variables cannot be used in the illustrated use case, merely that in this example they were not populated.
 14. The following Qualifiers would generally not be used in DT: --BODSYS, --LOC, --SER,--ACN,--ACNOTH, --REL, --RELNST, --PATT, --OUT, --SCAN, --SCONG, --SDISAB, --SDTH, --SHOSP, --SLIFE, --SOD, --SMIE, --CONTRT, --TOX, -TOXGR.

4.5.2 Examples for the Device Tracking and Disposition Domain Model

Example 1: These examples show individual device tracking at each change of location.

Rows 1 and 2: Device S001 was shipped to the site and implanted in the subject, where it is at the time of reporting. The device could be an orthopedic rod.

Rows 3 - 5: Device was shipped to Site 01, then it was returned to the sponsor, and then the same device was shipped to Site 02. The device could be a diagnostic tool that is used on multiple subjects, and then redeployed when the first site has completed their use of it.

Row 6: Device was shipped to the site but no further activity has happened.

Row 7 - 10: Device was shipped to the site, implanted in a subject, and then explanted and returned to the sponsor.

CDISC Study Data Tabulation Model Implementation Guide for Medical Devices Version 1.0

Rows 11-14: Device was shipped to the site and implanted in subject. Subsequently, the device was explanted and destroyed by site personnel.

Rows 15 – 17: The device, a tympanostomy tube, was shipped to the site and implanted in a subject. After the subject returned home, the tube dislodged and was lost.

Row	STUDYID	DOMAIN	SPDEVID	DTSEQ	DTTERM	DTDECOD	DTPARTY	DTPRTYID	DTCAT	DTDTC	DTSTDTC
1	ABC-123	DT	S001	1	Shipped	SHIPPED	SITE	02		2010-06-25	2010-06-25
2	ABC-123	DT	S001	2	Implantation	IMPLANTED	SUBJECT	02-1024		2010-07-15	2010-06-30
3	ABC-123	DT	S002	1	Shipped	SHIPPED	SITE	01		2010-11-03	2010-11-03
4	ABC-123	DT	S002	2	Returned	SHIPPED	SPONSOR			2011-01-05	2011-01-05
5	ABC-123	DT	S002	3	Shipped	SHIPPED	SITE	02		2011-01-15	2011-01-15
6	ABC-123	DT	S003	1	Shipped	SHIPPED	SITE	05		2010-09-29	2010-09-29
7	ABC-123	DT	S004	1	Shipped	SHIPPED	SITE	04		2010-08-30	2010-08-30
8	ABC-123	DT	S004	2	Implanted	IMPLANTED	SUBJECT	04-1009		2010-11-05	2010-10-20
9	ABC-123	DT	S004	3	Explanted	EXPLANTED	SITE	04		2010-11-05	2010-11-01
10	ABC-123	DT	S004	4	Shipped	SHIPPED	SPONSOR			2010-11-02	2010-11-02
11	ABC-123	DT	S005	1	Shipped	SHIPPED	SITE	04		2010-11-01	2010-11-01
12	ABC-123	DT	S005	2	Implanted	IMPLANTED	SUBJECT	04-1009		2010-12-06	2010-11-12
13	ABC-123	DT	S005	3	Explanted	EXPLANTED	SITE	04		2010-12-06	2010-12-01
14	ABC-123	DT	S005	4	Destroyed	DESTROYED				2010-12-10	2010-12-09
15	ABC-123	DT	Z045-2	1	Shipped	SHIPPED	SITE	05		2010-12-06	2010-11-12
16	ABC-123	DT	Z045-2	2	Implanted	IMPLANTED	SUBJECT	05-5005		2010-11-12	2010-11-16
17	ABC-123	DT	Z045-2	3	Lost	LOST				2010-11-18	2010-11-17

Example 2: Implantable Device - Disposition Usage Only

Row	STUDYID	DOMAIN	SPDEVID	DTSEQ	DTTERM	DTDECOD	DTPARTY	DTPRTYID	DTCAT	DTDTC	DTSTDTC
1	ABC-123	DT	S001	1	Implanted	IMPLANTED	SUBJECT	02-1024		2010-07-15	2010-06-30
2	ABC-123	DT	S002	2	Shipped	SHIPPED	SITE	02		2011-01-15	2011-01-15
3	ABC-123	DT	S003	3	Shipped	SHIPPED	SITE	05		2010-09-29	2010-09-29
4	ABC-123	DT	S004	4	Shipped	SHIPPED	SPONSOR			2010-11-02	2010-11-02
5	ABC-123	DT	S005	5	Destroyed	DESTROYED				2010-12-10	2010-12-09
6	ABC-123	DT	Z045-2	6	Lost	LOST				2010-11-18	2010-11-17

Example 3: Spray-On Skin - Disposition Usage Only

These rows show the tracking of a two part spray gun for applying skin cells to burns.

Rows 1 and 3: The spray gun body is sent to the site and returned to the sponsor.

Rows 2 - 4: The disposable cartridge that holds the cells is shipped to the site, and then destroyed after use.

Row	STUDYID	DOMAIN	SPDEVID	DTSEQ	DTTERM	DTDECOD	DTPARTY	DTPRTYID	DTDTC	DTSTDTC
1	Z937m	DT	SSG124	1	Shipped	SHIPPED	SITE	01	2011-06-29	2011-06-29
2	Z937m	DT	SSC2160	2	Shipped	SHIPPED	SITE	01	2011-06-29	2011-06-29
3	Z937m	DT	SSG124	3	Shipped	SHIPPED	SPONSOR		2011-08-30	2011-08-30
4	Z937m	DT	SSC2160	4	Destroyed	DESTROYED			2011-07-05	2011-07-05

4.6 DEVICE-SUBJECT RELATIONSHIPS - DR

dr.xpt, Response - Special Purpose Version 1.0. One record per device/subject combination,

Variable Name	Variable Label	Type	Controlled Terms, Code list or Format	Role	Definition	Implementation Notes	Core
STUDYID	Study Identifier	Char		Identifier	Unique identifier for a study.	Unique identifier for a study.	Req
DOMAIN	Domain Abbreviation	Char	DR	Identifier	Two-character abbreviation for the domain.	Two-character abbreviation for the domain.	Req
USUBJID	Unique Subject Identifier	Char		Identifier	Identifier used to uniquely identify a subject across all studies for all applications or submissions involving the product.	Required as the purpose of this domain is to link each USUBJID to one or more devices.	Req
SPDEVID	Sponsor Device Identifier	Char		Identifier	Sponsor-defined identifier for the device	It must be unique for each tracked unit of the device under study, and can be at whatever level of granularity the device should be identified (e.g., model or serial number, or combination of identifiers) as defined in DI.	Req

4.6.1 Assumptions for the Device-Subject Relationships Domain Model

1. The Device-Subject Relationships domain is a special-purpose domain that links each subject to the associated devices.
2. Information in this table may have been initially collected and submitted in other domains (e.g., Device Exposure, Device Tracking and Disposition, Device Events). This domain, however, provides a single, consistent location to find the relationship between a subject and a device, regardless of the device or the domain in which subject-related data may have been collected or submitted.
3. This domain is a special purpose domain and does not have a topic variable.
4. This domain allows for many-to-many relationships such that a single subject may be associated with several devices (for example, blood glucose test meters), a single device or class of devices may be associated with several subjects (for example, an MRI machine), or several devices may be associated with several subjects. In effect, this creates an index of the device/subject associations that permits other domains to determine the correct associations without having to store all relationship data in every domain.
5. Sponsors are responsible for defining SPDEVID such that device-subject relationships are described with the necessary level of detail for the submission.

4.6.2 Examples for the Device-Subject Relationships Domain Model

Example 1: Generic MRI settings at imaging encounters

In this example, the study requires collection of MRI data at specified time intervals. The MRI equipment is not under study; the product under investigation may not even be a device. The study protocol requires collection of specific settings on the MRI equipment at each encounter, but there is no requirement to track the specific MRI machine(s) with which subjects were scanned.

Row	STUDYID	DOMAIN	USUBJID	SPDEVID
1	ABC-123	DR	101	MRI
2	ABC-123	DR	103	MRI
3	ABC-123	DR	201	MRI
4	ABC-123	DR	202	MRI

Example 2: Collection of Pacemaker settings

In this example, the study protocol requires that some subjects be implanted with a pacemaker prior to enrollment, while others are not. The pacemakers are not under study; the product under investigation may not even be a device. The study protocol requires analysis stratified by whether or not subjects have a pacemaker, and if they do, the type of pacemaker (single- or dual-chamber) they have. There is no requirement to track the specific pacemaker implanted in each subject. At some point during the study, subject C13 has a single chamber pacemaker replaced with a dual chamber model. Information on when and why this happened would not be discernible from DR, but could be captured in DX.

Row	STUDYID	DOMAIN	USUBJID	SPDEVID
1	ABC-456	DR	A11	Dual Chamber Pacemaker
2	ABC-456	DR	A12	Dual Chamber Pacemaker
3	ABC-456	DR	B21	Single Chamber Pacemaker
4	ABC-456	DR	C13	Single Chamber Pacemaker
5	ABC-456	DR	C13	Dual Chamber Pacemaker

Example 3: Approval of Coronary Stent and Delivery Catheter

In this example, a new coronary stent and delivery catheter system is being submitted for approval to market. Delivery catheters are tracked by manufacturing lot; stents are tracked by individual unit serial number.

Subject 103 was exposed to 2 investigational stents, but the Device-Subjects Relationship table provides no further information.

On Row 10, Subject 202 had an adverse event during the PCI procedure that was related to the Venotrate Introducer (a tool used in the procedure). The Device-Subject Relationships table captures the relationship between the subject and the device, but all additional information about the AE would be captured in the AE domain.

Row	STUDYID	DOMAIN	USUBJID	SPDEVID
1	STUDY42	DR	101	Lot EZN123
2	STUDY42	DR	101	S/N BBS1001
3	STUDY42	DR	103	Lot EZN123
4	STUDY42	DR	103	S/N BBS1045
5	STUDY42	DR	103	S/N BBS1047
6	STUDY42	DR	201	Lot EZN201
7	STUDY42	DR	201	S/N BBS1067
8	STUDY42	DR	202	Lot EZN217
9	STUDY42	DR	202	S/N BBS1012
10	STUDY42	DR	202	Lot VI321

4.7 DEVICE PROPERTIES - DO

do.xpt, Device Properties - Findings, Version 1.0 One record per property per device, Tabulation

Variable Name	Variable Label	Type	Controlled Terms, Codelist or Format	Role	Definition	Implementation Notes	Core
STUDYID	Study Identifier	Char		Identifier	Unique identifier for a study.		Req
DOMAIN	Domain Abbreviation	Char	DO	Identifier	Two-character abbreviation for the domain.		Req
SPDEVID	Sponsor Device Identifier	Char		Identifier	Sponsor-defined identifier for the device.	It must be unique for each tracked unit of the device under study, and can be at whatever level of granularity the device should be identified (e.g., model or serial number, or combination of identifiers).	Req
DOSEQ	Sequence Number	Num		Identifier	Sequence Number given to ensure uniqueness of device records within subject records within a domain.	May be any valid number. It should be unique within every subject/device combination.	Req
DOGRPID	Group ID	Char		Identifier	Used to tie together a block of related records in a single domain for a device.		Perm
DORFID	Reference ID	Char		Identifier	Internal or external identifier.	This could be a scan code or equivalent.	Perm
DOSPID	Sponsor-Defined Identifier	Char		Identifier	Sponsor-defined reference number.		Perm
DOTESTCD	Device Property Short Name	Char	(DOTESTCD) *	Topic	Short name of the measurement, test, or examination described in DOTEST.	It can be used as a column name when converting a dataset from a vertical to a horizontal format. The value in DOTESTCD cannot be longer than 8 characters, nor can it start with a number (e.g. "1TEST"). DOTESTCD cannot contain characters other than letters, numbers, or underscores. Examples: LIFE, INDICATN, COMPOS	Req
DOTEST	Device Property Test Name	Char	(DOTEST)	Synonym Qualifier	Verbatim name of the test or examination used to obtain the measurement or finding.	The value in DOTEST cannot be longer than 40 characters. Examples: Shelf Life, Indication (of disease), Composition (of device)	Req
DOCAT	Category for Device In-Use	Char	*	Grouping Qualifier	Defines a category of related records.	For example, it can be used to define the type of property being defined, such as DIMENSIONS vs. MATERIAL	Perm
DOSCAT	Subcategory for Device In-Use	Char	*	Grouping Qualifier	A further categorization of a measurement or examination	For example, if DOCAT = DIMENSION, DOSCAT might be LENGTH or WIDTH or THICKNESS	Perm
DOORRES	Result or Finding in Original Units	Char		Result Qualifier	Result of the Device Property as originally observed or collected.	DOORRES should contain the result or value of the property defined in DOTEST. For example, if DOTEST is LIFE (shelf life) then DOORRES might be 6 (months).	Exp

DOORRESU	Original Units	Char	(UNIT)	Variable Qualifier	Original units in which the data were collected.	The unit for DOORRES. Examples: MONTHS, cm	Exp
----------	----------------	------	--------	--------------------	--	--	-----

* Indicates variable may be subject to controlled terminology; sponsor will identify the controlled terminology in define.XML.

4.7.1 Assumptions for the Device Properties Domain Model

1. Device Properties (DO): This Findings domain defines important characteristics of a device that the sponsor wishes to include in the submission but that *do not form part of the unique sponsor-defined identification of the device*. If there are no non-identifier characteristics to submit, this domain may not be necessary.
2. Each property is identified using controlled terminology and is stored in DOTESTCD/DOTEST, which allows the property names to be values in DOTESTCD in an SDTM-based vertical (normalized) structure and variable names in a CDASH horizontal (non-normalized) structure, if necessary. The controlled terminology has not yet been identified.
3. There should be one record per device property.
4. Sponsors define the properties and levels of granularity that are appropriate to include in this domain.
5. DO supports all device types (e.g., implantable, imaging, diagnostic), although implementation may vary by device type.
6. This domain does not define the relationships between tracked components and the overall device. This will be addressed in a future version of the standard.
7. DO should not contain characteristics that may change during the course of the study for a given device, such as dial settings on an imaging machine or software versions. As a result, the domain does not include Timing variables (SDTM Table 2.2.5).
8. Sponsors may choose whether to include characteristics in DO of approved products or components that are used in the study in accordance with the approved labeling.
9. The DO domain can contain data about devices that were not deployed, as there is no subject identifier in DO. It should contain only data that should be submitted with the clinical data; additional manufacturing and quality data may exist elsewhere in the submission and do not need to be included in DO unless the sponsor has a specific reason to do so.
10. DO data would generally be assembled by a sponsor, rather than by an investigative site. The data can be captured using a case report form, assembled on a worksheet to support entry of the information into the clinical database, derived manually or derived electronically from data in other domains or elsewhere.
11. DOTESTCD values are limited to 8 characters and cannot begin with a number or underscore as they can be used as variable names when the dataset is transposed to a non-normalized structure.
12. Note that in some of the examples below, variables that would be blank may have been dropped to conserve space. This does not mean that the variables cannot be used in the illustrated use case, merely that in this example they were not populated.
13. The following Qualifiers would not generally be used in DO: --MODIFY, --BODSYS, --POS,--ORNRL0, --ORNRLI, --STNRLO, --STNRHI, --STNRC, --NRIND, --RESCAT, --STAT, --REASND, --XFN, --NAM, --LOINC, --SPEC, --ANTREG, --SPCCND, --LOC, --LAT, --DIR, --METHOD, --LEAD, --BLFL, --FAST, --DRVFL, --EVAL, --TOX, --TOXGR, --SEV, --DTHREL and LLOQ

4.7.2 Examples for the Device Properties Domain Model

Example 1:

This example shows characteristics of 2 kinds of nylon mesh filter. The characteristics will not change, so the date is not relevant.

Row	STUDYID	DOMAIN	SPDEVID	DOSEQ	DOTESTCD	DOTEST	DOCAT	DOSCAT	DOORRES	DOORRESU
1	STUDYX	DO	ABC174	1	CLASS	Class	RISK PROFILE		3	
2	STUDYX	DO	ABC174	2	PORESIZE	Pore Size	DIMENSION		20	um
3	STUDYX	DO	ABC174	3	THCKNESS	Mesh Thickness	DIMENSION		52	um
4	STUDYX	DO	ABC174	4	OPENAREA	Mesh Open Area	DIMENSION		14	%
5	STUDYX	DO	ABC259	1	CLASS	Class	RISK PROFILE		3	
6	STUDYX	DO	ABC259	2	PORESIZE	Pore Size	DIMENSION		43	um
7	STUDYX	DO	ABC259	3	THCKNESS	Mesh Thickness	DIMENSION		35	um
8	STUDYX	DO	ABC259	4	OPENAREA	Mesh Open Area	DIMENSION		22	%

Example 2:

The two data points being conveyed to the regulators are the color of the kit box and the Lot ID of the kit’s reagents. In this case, the color is associated with the number of tests contained in the kit, with the red box containing 6 tests and the blue box containing 8 tests.

Row	STUDYID	DOMAIN	SPDEVID	DOSEQ	DOTESTCD	DOTEST	DOORRES	DOORRESU
1	ABC-125	DO	423-001	1	TESTNUM	Number of Tests	6	
2	ABC-125	DO	423-001	2	REAGLOT	Reagent Lot ID	123-56	
3	ABC-125	DO	876-523	1	TESTNUM	Number of Tests	8	
4	ABC-125	DO	876-523	2	REAGLOT	Reagent Lot ID	123-60	

5 CROSS-DOMAIN RELATIONSHIP EXAMPLES

5.1 DEVICE IN-USE AND TEST RESULTS

This section illustrates the way that Device In-Use (the settings of the device used) can be related to the results generated from the measurement or output of the device. This uses the example in the Device In-Use domain earlier in this document that shows settings on an MRI and relates it to Morphology results obtained from the MRI scan.

Example 1:

This example shows data from one subject collected at one visit about parameters from an MRI imaging protocol. It assumes the image was used for obtaining Morphology observations, as shown by the choice of DUGRPID. DUSPID can be used to link to MO records, as shown below. DUSPID happens to mirror DUSEQ but this will not always be the case, for example, if one subject is assigned more than one device.

Rows 1-7: Represent 7 example Device In-Use records collected at the screening visit for a given subject.

Rows 8-14: Represent 7 example Device In-Use records collected at the first treatment visit for the same subject.

du.xpt

Row	STUDYID	DOMAIN	USUBJID	SPDEVID	DUSEQ	DUGRPID	DUREFID	DUSPID	DUTESTCD	DUTEST	DUORRES	DUORRESU
1	STUDYX	DU	2324-P0001	ABC174	1	DUMO1	222333-444555	1	COILSTR	Coil Strength	1.5	T
2	STUDYX	DU	2324-P0001	ABC174	2	DUMO1	222333-444555	2	ANTPLANE	Anatomical Plane	CORONAL	
3	STUDYX	DU	2324-P0001	ABC174	3	DUMO1	222333-444555	3	STHICK	Slice Thickness	1	mm
4	STUDYX	DU	2324-P0001	ABC174	4	DUMO1	222333-444555	4	MATRIX	Matrix	256X256	
5	STUDYX	DU	2324-P0001	ABC174	5	DUMO1	222333-444555	5	SFTWRVER	Software Version	15.0	
6	STUDYX	DU	2324-P0001	ABC174	6	DUMO1	222333-444555	6	FLDVIEW	Field of View	24	cm
7	STUDYX	DU	2324-P0001	ABC174	7	DUMO1	222333-444555	7	RCBDWTH	Receiver Bandwidth	16	kHz
8	STUDYX	DU	2324-P0001	ABC174	8	DUMO2	444555-666777	1	COILSTR	Coil Strength	1.0	T
9	STUDYX	DU	2324-P0001	ABC174	9	DUMO2	444555-666777	2	ANTPLANE	Anatomical Plane	CORONAL	
10	STUDYX	DU	2324-P0001	ABC174	10	DUMO2	444555-666777	3	STHICK	Slice Thickness	2	mm
11	STUDYX	DU	2324-P0001	ABC174	11	DUMO2	444555-666777	4	MATRIX	Matrix	256X256	
12	STUDYX	DU	2324-P0001	ABC174	12	DUMO2	444555-666777	5	SFTWRVER	Software Version	15.1	

CDISC Study Data Tabulation Model Implementation Guide for Medical Devices Version 1.0

Row	STUDYID	DOMAIN	USUBJID	SPDEVID	DUSEQ	DUGRPID	DUREFID	DUSPID	DUTESTCD	DUTEST	DUORRES	DUORRESU
13	STUDYX	DU	2324-P0001	ABC174	13	DUMO2	444555-666777	6	FLDVIEW	Field of View	25	cm
14	STUDYX	DU	2324-P0001	ABC174	14	DUMO2	444555-666777	7	RCBDWTH	Receiver Bandwidth	16	kHz

Row	DUSTRESC	DUSTRESN	DUSTRESU	VISITNUM	VISIT	VISITDY	DUDTC	DUDY
1 (cont)	1.5	1.5	T	1	SCREENING	-7	2011-04-19	-7
2 (cont)	CORONAL			1	SCREENING	-7	2011-04-19	-7
3 (cont)	1	1	mm	1	SCREENING	-7	2011-04-19	-7
4 (cont)	256X256			1	SCREENING	-7	2011-04-19	-7
5 (cont)	15.0			1	SCREENING	-7	2011-04-19	-7
6 (cont)	24	24	cm	1	SCREENING	-7	2011-04-19	-7
7 (cont)	16	1	kHz	1	SCREENING	-7	2011-04-19	-7
8 (cont)	1.0	1.0	T	2	IMPLANTATION	1	2011-04-26	1
9 (cont)	CORONAL			2	IMPLANTATION	1	2011-04-26	1
10 (cont)	2	2	mm	2	IMPLANTATION	1	2011-04-26	1
11 (cont)	256X256			2	IMPLANTATION	1	2011-04-26	1
12 (cont)	15.1			2	IMPLANTATION	1	2011-04-26	1
13 (cont)	25	25	cm	2	IMPLANTATION	1	2011-04-26	1
14 (cont)	16	16	kHz	2	IMPLANTATION	1	2011-04-26	1

CDISC Study Data Tabulation Model Implementation Guide for Medical Devices Version 1.0

- Row 1-7:** Represent 6 possible organ measurement tests and 1 physician interpretation at a screening visit. This shows data reported in the original result and unit in MOORRES and MOORRESU and standardized in MOSTRESC, MOSTRESN, and MOSTRESU. It also shows the standard terminology for MOTESTCD and MOTEST. MOSPID can be used to capture the link to the device used to obtain the data listed in this table and referenced above in Table 1 (for example, the SPDEVID for the device that did the scan). MOREFID can hold the unique identifier for that specific scan and would link to the scan results in a different domain (not shown).
- Row 8 - 14** Represent the same data as Rows 1-7 but for Visit 2.
- Row 15-20:** Represent the same six tests run on a calibration sample (there are no interpretation or derived records for the calibration sample). The MOGRPID has been set to CALIBRATION to distinguish it from the subject tests.

mo.xpt

Row	STUDYID	DOMAIN	USUBJID	MOREFID	MOSEQ	MOSPID	MOGRPID	MOTESTCD	MOTEST	MOMETHOD	MOLOC	MOLAT
1	STUDYX	MO	2324-P0001	1234-5678	1	ABC174	DUMO1	TOTVOL	Total Volume	MRI	BRAIN	
2	STUDYX	MO	2324-P0001	1234-5678	2	ABC174	DUMO1	VOLUME	Volume	MRI	BRAIN, HIPPOCAMPUS	LEFT
3	STUDYX	MO	2324-P0001	1234-5678	3	ABC174	DUMO1	VOLUME	Volume	MRI	BRAIN, HIPPOCAMPUS	RIGHT
4	STUDYX	MO	2324-P0001	1234-5678	4	ABC174	DUMO1	VOLUME	Volume	MRI	TEMPORAL LOBE	LEFT
5	STUDYX	MO	2324-P0001	1234-5678	5	ABC174	DUMO1	VOLUME	Volume	MRI	TEMPORAL LOBE	RIGHT
6	STUDYX	MO	2324-P0001	1234-5678	6	ABC174	DUMO1	VOLUME	Volume	MRI	BRAIN, VENTRICLE	
7	STUDYX	MO	2324-P0001	1234-5678	7	ABC174	DUMO1	ABBSI	Annualized Brain Boundary Shift Int	MRI	BRAIN	
8	STUDYX	MO	2324-P0001	1234-5678	8	ABC174	DUMO2	TOTVOL	Total Volume	MRI	BRAIN	
9	STUDYX	MO	2324-P0001	1234-5678	9	ABC174	DUMO2	VOLUME	Volume	MRI	BRAIN, HIPPOCAMPUS	LEFT
10	STUDYX	MO	2324-P0001	1234-5678	10	ABC174	DUMO2	VOLUME	Volume	MRI	BRAIN, HIPPOCAMPUS	RIGHT
11	STUDYX	MO	2324-P0001	1234-5678	11	ABC174	DUMO2	VOLUME	Volume	MRI	TEMPORAL LOBE	LEFT
12	STUDYX	MO	2324-P0001	1234-5678	12	ABC174	DUMO2	VOLUME	Volume	MRI	TEMPORAL LOBE	RIGHT
13	STUDYX	MO	2324-P0001	1234-5678	13	ABC174	DUMO2	VOLUME	Volume	MRI	BRAIN, VENTRICLE	
14	STUDYX	MO	2324-P0001	1234-5678	14	ABC174	DUMO2	ABBSI	Annualized Brain Boundary Shift Int	MRI	BRAIN	
15	STUDYX	MO		4567-8901	1	ABC174	CALIBRATION	TOTVOL	Total Volume	MRI	BRAIN	
16	STUDYX	MO		4567-8901	2	ABC174	CALIBRATION	VOLUME	Volume	MRI	BRAIN, HIPPOCAMPUS	LEFT

CDISC Study Data Tabulation Model Implementation Guide for Medical Devices Version 1.0

Row	STUDYID	DOMAIN	USUBJID	MOREFID	MOSEQ	MOSPID	MOGRPID	MOTESTCD	MOTEST	MOMETHOD	MOLOC	MOLAT
17	STUDYX	MO		4567-8901	3	ABC174	CALIBRATION	VOLUME	Volume	MRI	BRAIN, HIPPOCAMPUS	RIGHT
18	STUDYX	MO		4567-8901	4	ABC174	CALIBRATION	VOLUME	Volume	MRI	TEMPORAL LOBE	LEFT
19	STUDYX	MO		4567-8901	5	ABC174	CALIBRATION	VOLUME	Volume	MRI	TEMPORAL LOBE	RIGHT
20	STUDYX	MO		4567-8901	6	ABC174	CALIBRATION	VOLUME	Volume	MRI	BRAIN, VENTRICLE	

Table 2 (cont.)

Row	MOORRES	MOORRESU	MOSTRESC	MOSTRESN	MOSTRESU	MOBLFL	MODRVFL	VISITNUM	VISIT	VISITDY	MODTC	MODY
1 (cont)	1120000	mm3	1120000	1120000	uL	Y		1	SCREENING	-7	2011-04-19	-7
2 (cont)	2725	mm3	2725	2725	uL	Y		1	SCREENING	-7	2011-04-19	-7
3 (cont)	2685	mm3	2685	2685	uL	Y		1	SCREENING	-7	2011-04-19	-7
4 (cont)	15635	mm3	15635	15635	uL	Y		1	SCREENING	-7	2011-04-19	-7
5 (cont)	15650	mm3	15650	15650	uL	Y		1	SCREENING	-7	2011-04-19	-7
6 (cont)	7505	mm3	7505	7505	uL	Y		1	SCREENING	-7	2011-04-19	-7
7 (cont)			-1.5	-1.5	%		Y	2	IMPLANTATION	1	2011-04-26	1
8 (cont)	1120000	mm3	1120000	1120000	uL			2	IMPLANTATION	1	2011-04-26	1
9 (cont)	2725	mm3	2725	2725	uL			2	IMPLANTATION	1	2011-04-26	1
10 (cont)	2685	mm3	2685	2685	uL			2	IMPLANTATION	1	2011-04-26	1
11 (cont)	15635	mm3	15635	15635	uL			2	IMPLANTATION	1	2011-04-26	1
12 (cont)	15650	mm3	15650	15650	uL			2	IMPLANTATION	1	2011-04-26	1
13 (cont)	7505	mm3	7505	7505	uL			2	IMPLANTATION	1	2011-04-26	1
14 (cont)			-1.5	-1.5	%		Y	2	IMPLANTATION	1	2011-04-26	1
15 (cont)	1130000	mm3	1130000	1130000	uL						2011-04-18	
16	2740	mm3	2740	2740	uL						2011-04-	

CDISC Study Data Tabulation Model Implementation Guide for Medical Devices Version 1.0

Row	MOORRES	MOORRESU	MOSTRESC	MOSTRESN	MOSTRESU	MOBLEFL	MODRVFL	VISITNUM	VISIT	VISITDY	MODTC	MODY
17 (cont)	2670	mm3	2670	2670	uL						18	
18 (cont)	15752	mm3	15752	15752	uL						2011-04-18	
19 (cont)	15685	mm3	15685	15685	uL						2011-04-18	
20 (cont)	7597	mm3	7597	7597	uL						2011-04-18	

Represents the RELREC relationship between *du.xpt* and *mo.xpt* above. Note that CALIBRATION, the MOGRPID value for the calibration run, does not appear here because there is no corresponding subject. See the SDTMIG (RELREC section) for further discussion and examples of RELREC.

relrec.xpt

Row	STUDYID	USUBJID	RDOMAIN	IDVAR	IDVARVAL	RELTYPE	RELID
1	STUDYX		MO	MOGRPID		MANY	MODU1
2	STUDYX		DU	DUGRPID		MANY	MODU1

6 APPENDICES

Appendix A: Glossary, Acronyms, and Definitions

The following abbreviations and terms may be used in this document. Additional definitions can be found in the CDISC Glossary available at <http://www.cdisc.org/glossary/index.html>.

Abbreviation / Acronym / Term	Definition
510(k)	A kind of regulatory submission in which a device company requests permission from the FDA to market a new device when the device is “substantially equivalent” in safety and efficacy to one that is already marketed. Such devices are generally seen as lower risk, and do not necessarily require clinical trials for FDA to clear them.
Ancillary Device	A device used within a clinical trial to collect subject data information (device or human subject), but that is not the target of the study (e.g., a MRI or CT machine whose settings must be recorded in the clinical trial data, as required in the protocol)
BLA	Biologics License Application: A submission made by the manufacturer of a licensed biologic that also meets the definition of a medical device and which is subsequently subjected to scientific review by CBER (or FDA) to determine the biologics/device’s safety, purity and potency and the acceptability of the manufacturing facilities before approval for marketing.
BRIDG	Biomedical Research Integrated Domain Group
caBIG	cancer B iomedical I nformatics G rid™. An information network enabling all constituencies in the cancer community – researchers, physicians, and patients – to share data and knowledge.
CBER	Center for Biologics Evaluation and Research, one of the divisions of the FDA responsible for regulatory evaluation of medical devices, among other responsibilities
CDASH	Clinical Data Acquisition Standards Harmonization Project. The name for the project that delivers basic data collection fields (this document)
CDISC	Clinical Data Interchange Standards Consortium, a Standards Development Organization
CDM	Clinical Data Management
CDRH	Center for Devices and Radiological Health, one of the divisions of the FDA responsible for regulatory evaluation of medical devices, among other responsibilities
Class I Device ¹	A device proposed for regulatory review that is perceived to be low risk. Requirements for clearance for marketing are “general controls” and include provisions that relate to adulteration; misbranding; device registration and listing; premarket notification; banned devices; notification, including repair, replacement, or refund; records and reports; restricted devices; and good manufacturing practices. Examples include elastic bandages, handheld surgical tools and examination gloves.
Class II Device ¹	Devices for which the controls for Class I are not considered sufficient to ensure safety and efficacy, and thus additional controls are required, which may include special labeling requirements, mandatory performance standards and other controls. Examples include powered wheelchairs, infusion pumps, and surgical drapes.
Class III Device ¹	A device for which Class I and Class II controls do not provide sufficient evidence for its safety and efficacy. These devices are generally of higher risk to humans. Examples include implantable pacemaker, pulse generators, HIV diagnostic tests, automated external defibrillators, and endosseous implants.
Collected	Within this document collected refers to information that is recorded and/or transmitted to the sponsor. This includes data entered by the site on CRFs/eCRFs as well as vendor data such as core lab data. This term is a synonym for “captured”.
Controlled Terminology	A finite set of values that represent the only allowed values for a data item. These values may be codes, text, or numeric. A code list is one type of controlled terminology.
CRF	Case report form (sometime case record form) A printed, optical, or electronic document designed to record all required information to be reported to the sponsor for each trial subject.
CTCAE	Common Terminology Criteria for Adverse Events
Databased	To have put (data) into a database.
Dataset	A collection of structured data in a single file
Derived	Within this document derived refers to information that is not directly entered into the specific data field by the investigator site or by a core lab. This category includes autoencoded data, calculated data and similar electronically generated data, but not prepopulated fields.
Domain	A collection of observations with a topic-specific commonality about a subject
eCRF	Electronic case report form
EMA	The European Medicines Agency. A decentralized body of the European Union, main responsibility is the protection and promotion of public and animal health, through the evaluation and supervision of medicines for human and veterinary use.
Epoch	Interval of time in the planned conduct of a study. An epoch is associated with a purpose (e.g., screening, randomization, treatment, follow-up), which applies across all arms of a study.
EVS	Enterprise Vocabulary Services
FAQs	Frequently Asked Questions

Abbreviation / Acronym / Term	Definition
FDA	Food and Drug Administration Part of the US Department of Health and Human Services Agency. The regulatory authority for all pharmaceuticals (including biologics and vaccines) and medical devices in the US.
GCDMP	Good Clinical Data Management Practices (GCDMP). SCDM publication on clinical data management processes
GCP	Good Clinical Practice
HL7	Health Level 7
ICH	International Conference on Harmonization of Technical Requirements for Registration of Pharmaceuticals for Human Use
ICH E2A	ICH guidelines on Clinical Safety Data Management: Definitions and Standards for Expedited Reporting
ICH E2B	ICH guidelines on Clinical Safety Data Management: Data Elements For Transmission Of Individual Case Safety Reports
ICH E2C	ICH guidelines on Clinical Safety Data Management: Periodic Safety Update Reports For Marketed Drugs
ICH E3	ICH guidelines on Structure and Content of Clinical Study Reports
ICH E4	ICH guidelines on Dose-response Information to Support Drug Registration
ICH E5	ICH guidelines on Ethnic Factors in the Acceptability of Foreign Clinical Data
ICH E6 (R1)	ICH guideline for Good Clinical Practice
ICH E9	ICH guidelines on Statistical Principles for Clinical Trials
ICH E11	ICH guidelines on Clinical Investigation of Medicinal Products in the Pediatric Population
ICH E14	ICH guidelines on the Clinical Evaluation Of QT/QTc Interval
IDE	Investigational Device Exemption - IDE application required by the US FDA before some clinical trials of a new medical device may be initiated.
IND	Investigational New Drug. IND application required by the US FDA before clinical trials of a new drug or new biological agent may be initiated.
IRB	Institutional Review Board. Under FDA regulations, an IRB is an appropriately constituted group that has been formally designated to review and monitor biomedical research involving human subjects
ISO 8601	International Organization for Standardization document of character representation of dates, date/times, intervals, and durations of time
Many-to-Many	Describes the relationship between two sets of objects (e.g., data points or observations in datasets) where each object in each dataset has a relationship with many objects in the other dataset. For example, one subject could have many medical history conditions (e.g., headache, toothache, earache), and a given medical history condition (e.g., headache) can be had by many subjects. See one-to-one and one-to-many.
MedDRA	Medical Dictionary for Regulatory Activities (new global standard medical terminology designed to supersede other terminologies (such as COSTART and ICD9) used in the medical product development process
NCI	National Cancer Institute (NIH)
NCI EVS	National Cancer Institute (NIH) Enterprise Vocabulary Services
NCRR	The National Clinical Research Resources, a Collaborative Group Member
NDA	New Drug Application
NICHHD	The National Institute of Child Health and Human Development, a Collaborative Group Member
NIH	National Institutes of Health
NLM	National Library of Medicine
ODM	Operational Data Model. Format for representing the study metadata, study data and administrative data associated with a clinical trial
One-to-One	Describes the relationship between two sets of objects (e.g., observations in datasets) where each object in each dataset has a relationship with one and only one object in the other dataset. For example, Subject 1 is assigned only Lab Kit 1, and Lab Kit 1 is assigned only to Subject 1. See many-to-many and one-to-many.
One-to-Many	Describes the relationship between two sets of objects (e.g., observations in datasets) where each object in one dataset has a relationship with many objects in the other dataset, but the objects in the second dataset each have only one relationship with one object in the first dataset. For example, Subject 1 could have many lab tests, but each lab test is assigned only Subject 1. See many-to-many and one-to-one.
OTC	Over The Counter.
PhRMA	Pharmaceutical Research and Manufacturers Association

CDISC Study Data Tabulation Model Implementation Guide for Medical Devices Version 1.0

Abbreviation / Acronym / Term	Definition
PMA ¹	Premarket Approval. A process of scientific review to ensure the device's safety and effectiveness that must be completed for FDA to consider permitting marketing of the device. Class III devices typically require PMAs.
PRBC	Packed Red Blood Cells
Predicate Device ²	A legally marketed device that serves as the basis for comparison for a new device in a 510(k) premarketing notification.
Preprinted (pre-printed)	Items that are part of the original printing on a paper CRF. For example the unit required for a response, such as "years" for an age question. These data may or may not be stored in the database.
Prepopulated (pre-populated)	Items that are part of the eCRF (or data collection device) that are not enterable/modifiable. (also see preprinted). These data are stored in the study database.
PRN	As Needed (Latin: <i>pro re nata</i>)
Protocol Deviation	A variation from processes or procedures defined in a protocol. Deviations usually do not preclude the overall evaluability of subject data for either efficacy or safety, and are often acknowledged and accepted in advance by the sponsor. NOTE: Good clinical practice recommends that deviations be summarized by site and by category as part of the report of study results so that the possible importance of the deviations to the findings of the study can be assessed. <i>Compare to protocol violation.</i> [See ICH E3]
Protocol Violation	A significant departure from processes or procedures that were required by the protocol. Violations often result in data that are not deemed evaluable for a per-protocol analysis, and may require that the subject(s) who violate the protocol be discontinued from the study. <i>Compare to protocol deviation.</i>
RCRIM	Regulated Clinical Research Information Management
RIM	Reference Information Model
SAP	Statistical Analysis Plan
SCDM	Society for Clinical Data Management,
SDS	Submission Data Standards. Also the name of the Team that created the SDTM and SDTMIG
SDO	Standards Development Organization
SDTM	Study Data Tabulation Model
SDTMIG	SDTM Implementation Guide. When written just like this, it represents the original SDTMIG, in which the experimental unit is a subject, as compared to SEND, for example, where the experimental unit is an animal.
SDTMIG-MD	SDTM Implementation Guide for Medical Device trials, where the experimental unit is the device.
SOCs	System Organ Class (from MedDRA)
Study Treatment	The drug, device, therapy, or process under investigation in a clinical trial which has an effect on outcome of interest in a study: e.g., health-related quality of life, efficacy, safety, pharmacoeconomics. <i>Synonyms: intervention, therapeutic intervention, medical product.</i>
TA	Therapeutic area
Uncoded	Not coded. Not having or showing a code.
UUID	Universally Unique Identifier
WHO	World Health Organization
WHO ART	World Health Organization Adverse Reaction Terminology (WHO-ART) has been developed over more than 30 years to serve as a basis for rational coding of adverse reaction terms.
WHO Drug	World Health Organization Drug Dictionary

1. Definitions drawn from the following sources, as quoted in Wikipedia "Medical Device" retrieved 31 Aug 2011.

"Device Classification". Medical Devices. U.S. Food and Drug Administration.

"TITLE 21--FOOD AND DRUGS: CHAPTER I--FOOD AND DRUG ADMINISTRATION: DEPARTMENT OF HEALTH AND HUMAN SERVICES: SUBCHAPTER H--MEDICAL DEVICES: PART 860 MEDICAL DEVICE CLASSIFICATION PROCEDURES". CFR - Code of Federal Regulations Title 21. U.S. Food and Drug Administration.

"General and Special Controls". Medical Devices. U.S. Food and Drug Administration.

2. Definition drawn from the FDA's Medical Device page on "How to find a predicate device"

<http://www.fda.gov/MedicalDevices/DeviceRegulationandGuidance/HowtoMarketYourDevice/PremarketSubmissions/PremarketNotification510k/ucm134571.htm> retrieved 31 Aug 2011.

Appendix B: Supplemental Information

Appendix B1: Normalization of Data Structures

The following information describes the two primary data structures most often encountered in medical device trials, which are normalized (or vertical) and non-normalized (or horizontal). SDTM findings domain data (e.g., vital signs, ECG and Labs) are typically structured as normalized data. This allows for more flexible data for transmission to regulatory authorities. Data capture and many data analyses are easier when the data are in a non-normalized or horizontal format. This document presents examples of both formats for each findings domain. All other CDISC domains (i.e. special domains, interventions and events) are non-normalized or horizontal structures.

A non-normalized data table is more horizontal and may be easier to understand, while a normalized data table is more vertical and has properties that allow for database consistency during updates, inserts and deletes, and a simpler structure during queries. The rows of a normalized table will repeat items in its columns as needed in order to create a unique key for each row.

Typically, a table is called “normalized” if the data in it are in “third normal form”. First normal form requires that attributes (columns) be identifiable atomic values, rather than a group of values, such as a free entry text string containing date, blood pressure, and pulse. Second normal form requires a key that uniquely identifies each row in the table. In third normal form, all attributes identified by the key for the row are data elements that can be uniquely identified by the key. Even if pulse measurements are the same value on different days (e.g., 80 bpm), each entry represents an actual measurement.

An example of a non-normalized table would have a row for each subject and a column for each of a series of blood pressure measurements, creating a wide table. Each row would be updated multiple times, as each study visit required vital signs to be recorded, and the number of possible columns would be pre-defined. It would be easy for a human to read across such a table and identify a trend in blood pressure. Another example of a horizontal table would be one that had a subject, a date, a visit number, and a series of vital signs and blood test values in each row. Again, it may be easier for a human reader to understand data in this form and draw clinical conclusions. However, automated queries of such data may be more difficult.

In a normalized table, each row would contain a subject id, date, vital sign type (e.g., blood pressure), and the value recorded. With such a table, subject ID may be repeated many times, but the key consisting of subject ID, blood pressure, and date would be sufficient to identify a unique blood pressure measurement. It would be easy to add more measurements to such a table, for example, if the study is extended for follow-up. Also, other vital signs measurements can easily be added to this table, simply by using a different vital sign type (e.g., pulse). At each visit, a single row would be added for a vital sign type. This is the format used by the Findings domains in SDTM.

Appendix B2: CDISC Controlled Terminology

Terminology applicable to CDISC Device collection and submission fields is either in production or under development by the CDISC Terminology Team. Production terminology is published by the National Cancer Institute’s Enterprise Vocabulary Services (NCI EVS) and can be accessed via the following link: <http://www.cancer.gov/cancertopics/terminologyresources/CDISC>.

In cases where a CDISC Device field has associated controlled terminology, the code list is referenced in the Definition column in the domain tables.

Appendix C: Other Relevant Standards

Beyond those listed here, additional standards that may affect device clinical trials can be found on the FDA CDRH website at <http://www.fda.gov/MedicalDevices/DeviceRegulationandGuidance/Standards/default.htm>.

Appendix C1: Unique Device Identifier (UDI)

The FDA Amendments Act of 2007 (signed into law on September 27, 2007) mandated a physical label on devices, which called the “unique device identifier” or UDI. The labels will have two components:

Device Identifier: manufacturer, make and model

Production Identifier: serial or lot number and expiration date

Guidelines on the UDI have been published and are available at www.fda.gov/cdrh/ocd/udi. To find the UDI attributes, go to <http://www.ghtf.org/documents/ahwg/AHWG-UDI-N2R3.pdf>.

The UDI is intended to track individual device units once they are in the marketplace, and the information to be included is largely only obtainable after manufacture for distribution. As a result, most studies using this SDTM Implementation Guide will be unlikely to require UDIs. If needed, the UDI can be included as a characteristic in Device Identifiers (DI).

Appendix C2: Code of Federal Regulations

The primary US federal regulations affecting medical devices that have an impact on the capture and submission of clinical trials data to regulatory authorities are:

- 21 CFR Part 601 Licensing <http://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfcfr/CFRSearch.cfm?CFRPart=601>
- 21 CFR Part 660 - Additional Standards for Diagnostic Substances for Laboratory Tests <http://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfcfr/CFRSearch.cfm?CFRPart=660>
- 21 CFR Part 812 Investigational Device Exemptions <http://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfcfr/CFRSearch.cfm?CFRPart=812&showFR=1>
- 21 CFR Part 807 ESTABLISHMENT REGISTRATION AND DEVICE LISTING FOR MANUFACTURERS AND INITIAL IMPORTERS OF DEVICES, Subpart E Premarket Notification Procedures

<http://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfcfr/CFRSearch.cfm?CFRPart=807&showFR=1&subpartNode=21:8.0.1.1.5.5>

- 21 CFR Part 814 Premarket Approval of Medical Devices

<http://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfcfr/cfrsearch.cfm?cfrpart=814>

- 21 CFR Part 803 Medical Device Reporting

<http://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfcfr/CFRSearch.cfm?CFRPart=803>

Appendix C3: International Organization for Standardization (ISO)

The ISO 14155 standard was first developed in 2003 and recently update in 2011. This standard "addresses good clinical practice for the design, conduct, recording and reporting of clinical investigations carried out in human subjects to assess the safety or performance of medical devices for regulatory purposes." The following sections of the ISO 14155 relate to this CDISC Device standard:

- CRFs
- Device deficiencies
- Investigational device accountability

Appendix C4: Code Lists and Terminology

Beyond those defined by CDISC and managed by the NCI EVS (see Appendix A2 above), the following code lists and controlled terminologies may affect the structure and content of clinical data:

- Product Code Classification Database
<http://www.fda.gov/MedicalDevices/DeviceRegulationandGuidance/Overview/ClassifyYourDevice/ucm051637.htm>
- Event Problem Codes
<http://www.fda.gov/MedicalDevices/Safety/ReportaProblem/EventProblemCodes/default.htm>

Appendix D: Participating Companies

Leadership Team	Company affiliation
Carey Smoak	Roche Molecular Systems, Inc.
Kit Howard	Kestrel Consultants
Fred Wood	Octagon Research Solutions
Rhonda Facile	CDISC
Bob Pearsall	Axon
Maureen Lyden	BioStat Inc
Paul Franson	Medtronic, Inc.
Jennifer Duggan	St. Jude Medical
Marc Mucatel	WL Gore
Parag Shiralkar	Independent Consultant
Jennie Tedrow	Boston Scientific

Additional Participating Companies, Agencies and Institutions

Abbott	Edwards Lifesciences
AdvaMed	FDA-CBER
Alcon Labs	FDA-CDER
Allergan	FDA-CDRH
Bayer	Genprobe
Becton Dickinson	Harvard Clinical Research Institute
BioClinica	Innoventz
Biomet	Johnson & Johnson
Buckler Biomedical Sciences	National Cancer Institute
Business Bridge	PRA International
CDISC	Premier Research
Cleveland Clinic	Smith & Nephew
Covidien	Stryker
Dexcom	Synteract
eClinical Solutions	Trireme Medical

Appendix E: Representations and Warranties, Limitations of Liability, and Disclaimers

CDISC Patent Disclaimers

It is possible that implementation of and compliance with this standard may require use of subject matter covered by patent rights. By publication of this standard, no position is taken with respect to the existence or validity of any claim or of any patent rights in connection therewith. CDISC, including the CDISC Board of Directors, shall not be responsible for identifying patent claims for which a license may be required in order to implement this standard or for conducting inquiries into the legal validity or scope of those patents or patent claims that are brought to its attention.

Representations and Warranties

Each Participant in the development of this standard shall be deemed to represent, warrant, and covenant, at the time of a Contribution by such Participant (or by its Representative), that to the best of its knowledge and ability: (a) it holds or has the right to grant all relevant licenses to any of its Contributions in all jurisdictions or territories in which it holds relevant intellectual property rights; (b) there are no limits to the Participant's ability to make the grants, acknowledgments, and agreements herein; and (c) the Contribution does not subject any Contribution, Draft Standard, Final Standard, or implementations thereof, in whole or in part, to licensing obligations with additional restrictions or requirements inconsistent with those set forth in this Policy, or that would require any such Contribution, Final Standard, or implementation, in whole or in part, to be either: (i) disclosed or distributed in source code form; (ii) licensed for the purpose of making derivative works (other than as set forth in Section 4.2 of the CDISC Intellectual Property Policy ("the Policy")); or (iii) distributed at no charge, except as set forth in Sections 3, 5.1, and 4.2 of the Policy. If a Participant has knowledge that a Contribution made by any Participant or any other party may subject any Contribution, Draft Standard, Final Standard, or implementation, in whole or in part, to one or more of the licensing obligations listed in Section 9.3, such Participant shall give prompt notice of the same to the CDISC President who shall promptly notify all Participants.

No Other Warranties/Disclaimers. ALL PARTICIPANTS ACKNOWLEDGE THAT, EXCEPT AS PROVIDED UNDER SECTION 9.3 OF THE CDISC INTELLECTUAL PROPERTY POLICY, ALL DRAFT STANDARDS AND FINAL STANDARDS, AND ALL CONTRIBUTIONS TO FINAL STANDARDS AND DRAFT STANDARDS, ARE PROVIDED "AS IS" WITH NO WARRANTIES WHATSOEVER, WHETHER EXPRESS, IMPLIED, STATUTORY, OR OTHERWISE, AND THE PARTICIPANTS, REPRESENTATIVES, THE CDISC PRESIDENT, THE CDISC BOARD OF DIRECTORS, AND CDISC EXPRESSLY DISCLAIM ANY WARRANTY OF MERCHANTABILITY, NONINFRINGEMENT, FITNESS FOR ANY PARTICULAR OR INTENDED PURPOSE, OR ANY OTHER WARRANTY OTHERWISE ARISING OUT OF ANY PROPOSAL, FINAL STANDARDS OR DRAFT STANDARDS, OR CONTRIBUTION.

Limitation of Liability

IN NO EVENT WILL CDISC OR ANY OF ITS CONSTITUENT PARTS (INCLUDING, BUT NOT LIMITED TO, THE CDISC BOARD OF DIRECTORS, THE CDISC PRESIDENT, CDISC STAFF, AND CDISC MEMBERS) BE LIABLE TO ANY OTHER PERSON OR ENTITY FOR ANY LOSS OF PROFITS, LOSS OF USE, DIRECT, INDIRECT, INCIDENTAL, CONSEQUENTIAL, OR SPECIAL DAMAGES, WHETHER UNDER CONTRACT, TORT, WARRANTY, OR OTHERWISE, ARISING IN ANY WAY OUT OF THIS POLICY OR ANY RELATED AGREEMENT, WHETHER OR NOT SUCH PARTY HAD ADVANCE NOTICE OF THE POSSIBILITY OF SUCH DAMAGES.

Note: The CDISC Intellectual Property Policy can be found at http://www.cdisc.org/about/bylaws_pdfs/CDISCIPPolicy-FINAL.pdf.